

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL100121\
 Data File : VL037743.D
 Acq On : 1 Oct 2021 16:02
 Operator : SY/AP
 Sample : M4012-01 10X
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 C0P23DL

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 3
 Start Thrs: 0.001
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL091621AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Sep 16 13:42:46 2021

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.867	13	25	60	rBV	3509305	7507694	62.82%	11.982%
2	3.201	119	129	141	rBV2	298638	487745	4.08%	0.778%
3	3.594	239	251	275	rBV	1487883	3762434	31.48%	6.005%
4	3.841	318	328	349	rBV2	629584	1294309	10.83%	2.066%
5	3.960	355	365	383	rBV	280412	634789	5.31%	1.013%
6	4.333	466	481	504	rBV2	1524536	3021353	25.28%	4.822%
7	5.655	879	892	916	rBV4	2712971	6703597	56.09%	10.699%
8	7.160	1345	1360	1399	rBV	4764034	10702690	89.55%	17.081%
9	7.459	1439	1453	1466	rBV4	100694	234807	1.96%	0.375%
10	8.124	1647	1660	1670	rBV5	73414	166942	1.40%	0.266%
11	10.417	2361	2373	2379	rBV7	69035	130490	1.09%	0.208%
12	11.677	2750	2765	2782	rBV3	164444	444557	3.72%	0.710%
13	12.063	2868	2885	2913	rBV2	4814992	11951994	100.00%	19.075%
14	14.394	3591	3610	3631	rBV2	4428864	11562850	96.74%	18.454%
15	14.465	3631	3632	3641	rVB5	122342	143742	1.20%	0.229%
16	16.960	4390	4408	4429	rBV	986540	2789543	23.34%	4.452%
17	17.921	4691	4707	4708	rBV6	84503	138848	1.16%	0.222%
18	18.336	4818	4836	4847	rBV6	115275	315812	2.64%	0.504%
19	21.464	5791	5809	5810	rBV	213682	351910	2.94%	0.562%
20	21.471	5810	5811	5829	rVB2	192877	311304	2.60%	0.497%


Sum of corrected areas: 62657410

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL100121\
Data File : VL037743.D
Acq On : 1 Oct 2021 16:02
Operator : SY/AP
Sample : M4012-01 10X
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P23DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL091621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Sep 16 13:42:46 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

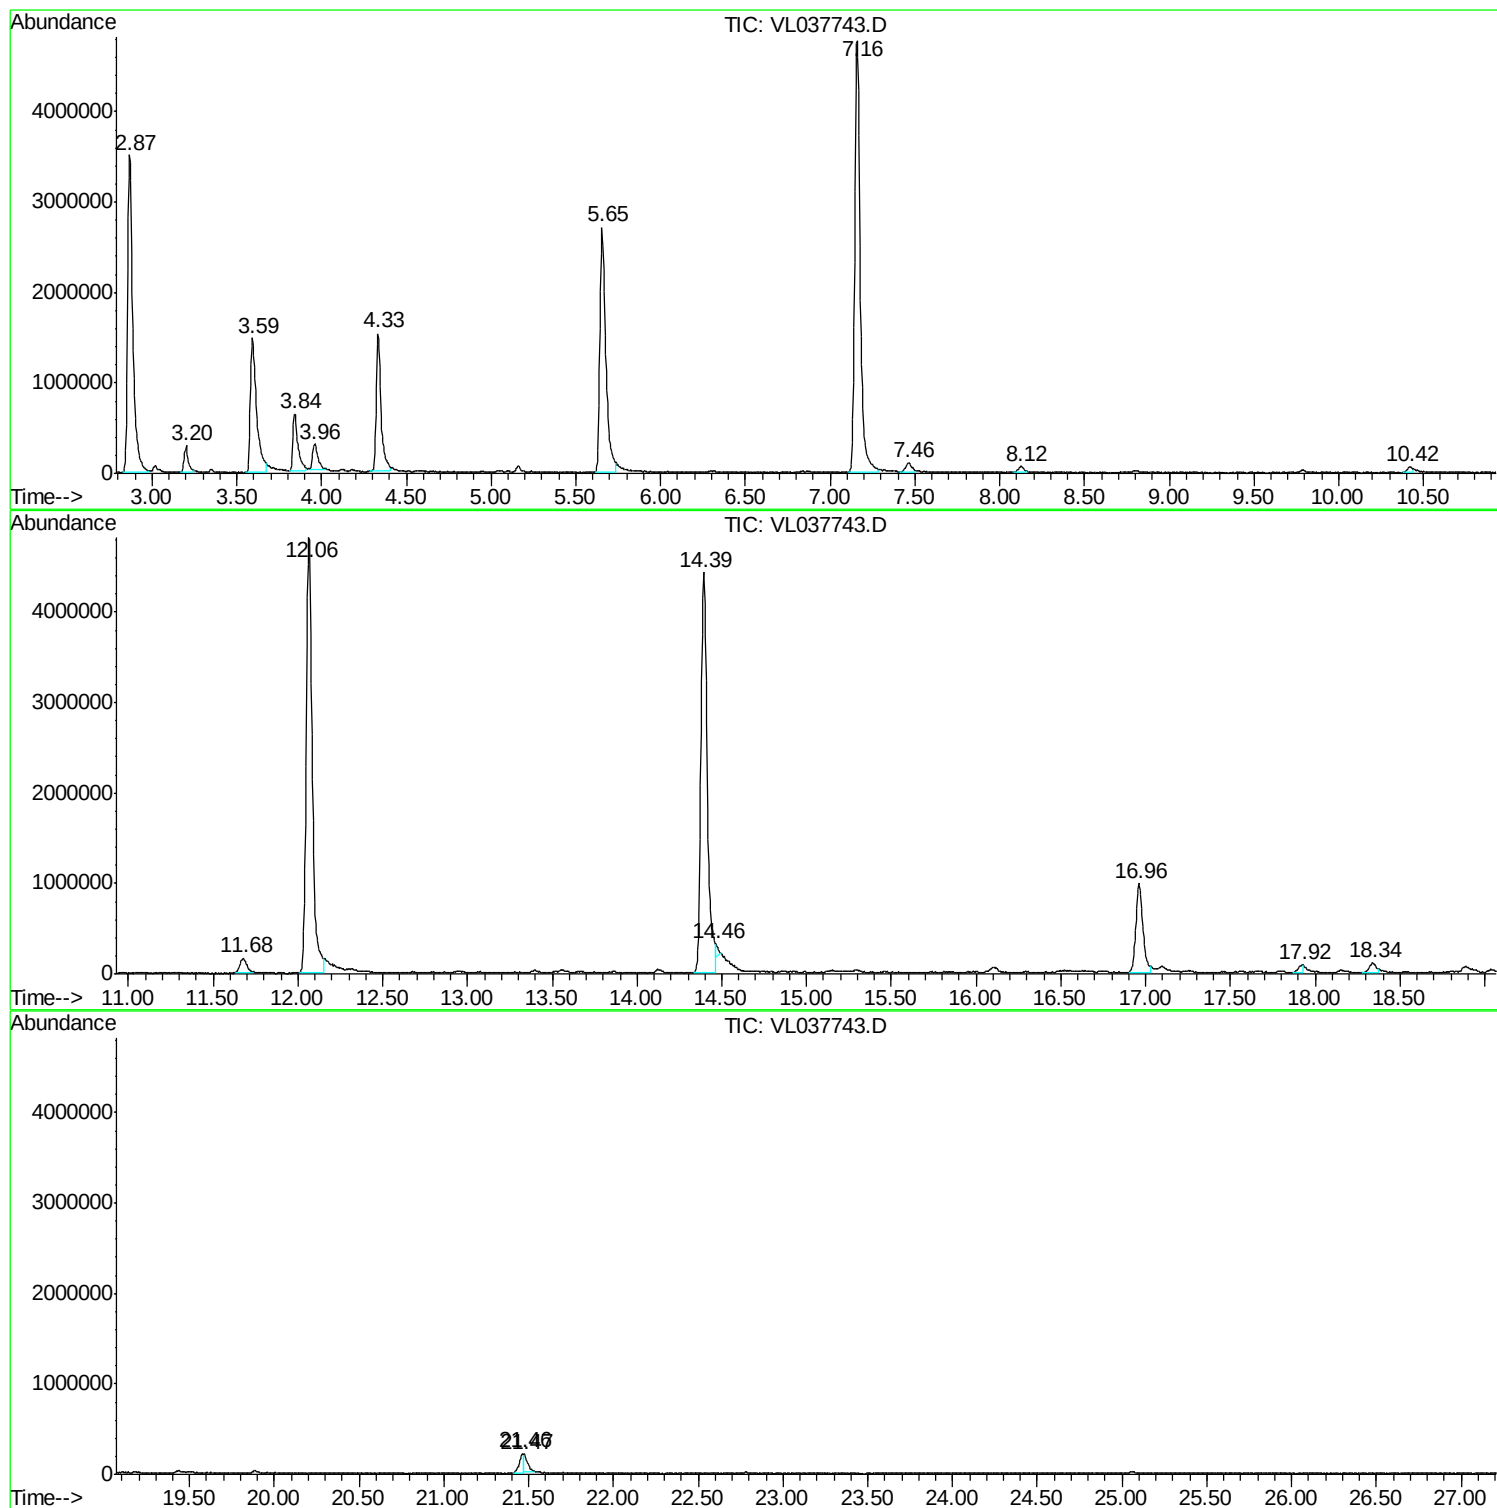

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL100121\
Data File : VL037743.D
Acq On : 1 Oct 2021 16:02
Operator : SY/AP
Sample : M4012-01 10X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P23DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL091621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Sep 16 13:42:46 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL100121\
Data File : VL037743.D
Acq On : 1 Oct 2021 16:02
Operator : SY/AP
Sample : M4012-01 10X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P23DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Sep 16 13:42:46 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc