


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL100121\  
 Data File : VL037737.D  
 Acq On : 1 Oct 2021 9:12  
 Operator : SY/AP  
 Sample : BFB  
 Misc : 400mL/MSVOA L  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_L  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL091621AIR.M  
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Thu Sep 16 13:42:46 2021  
 Last Update : Thu Sep 16 13:42:46 2021

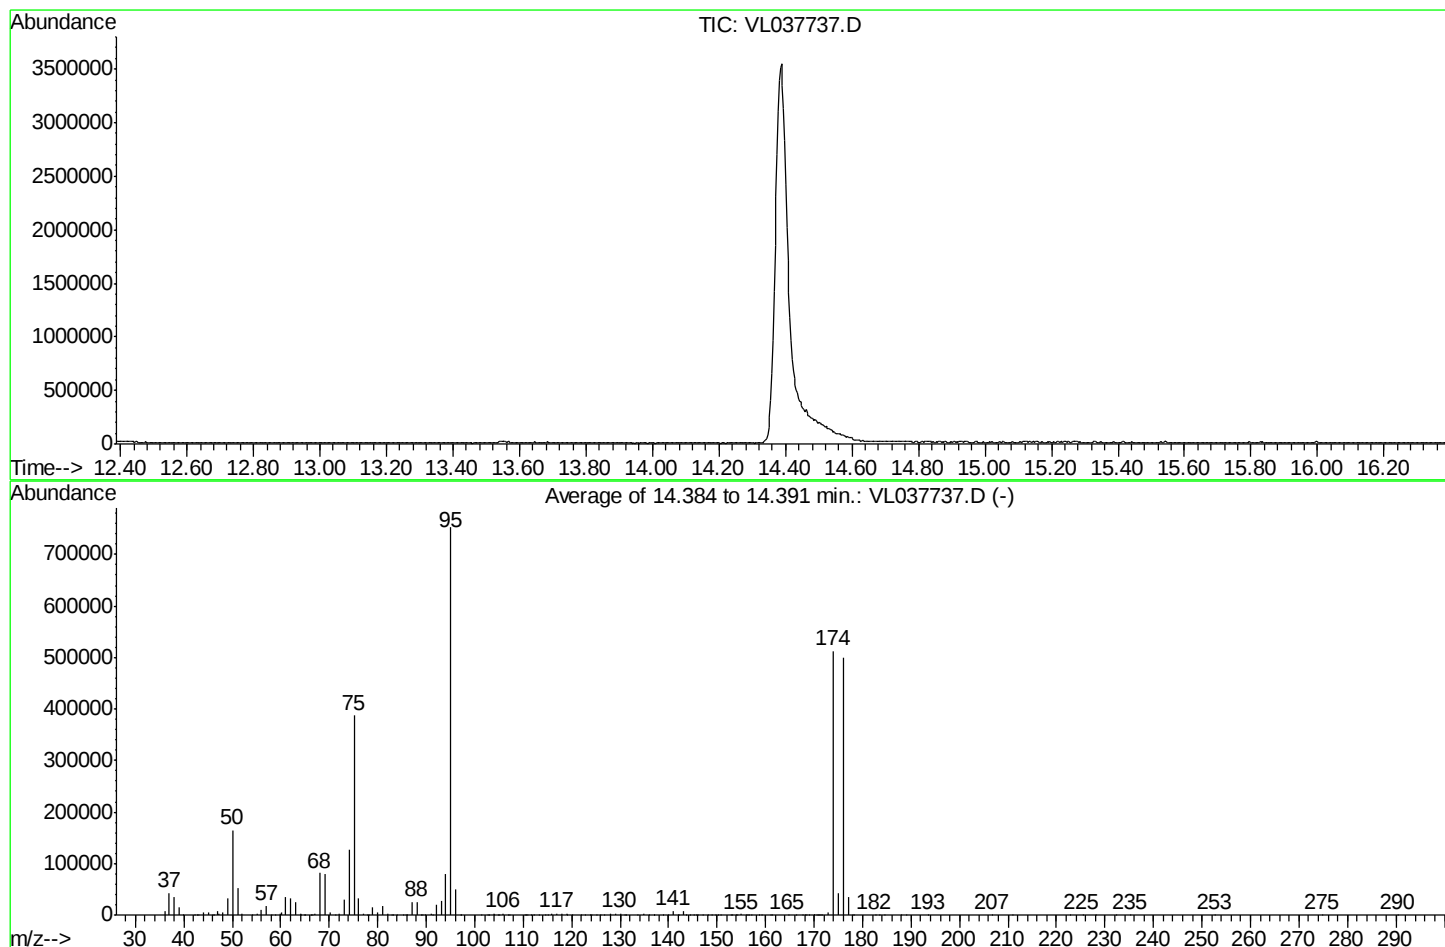

AutoFind: Scans 3607, 3608, 3609; Background Corrected with Scan 3585

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 8            | 40           | 21.9      | 164480  | PASS             |
| 75          | 95           | 30           | 66           | 51.5      | 387690  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 752725  | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 49994   | PASS             |
| 173         | 174          | 0.00         | 2            | 1.0       | 5267    | PASS             |
| 174         | 95           | 50           | 120          | 68.2      | 513130  | PASS             |
| 175         | 174          | 4            | 9            | 8.2       | 42176   | PASS             |
| 176         | 174          | 93           | 101          | 97.3      | 499200  | PASS             |
| 177         | 176          | 5            | 9            | 7.2       | 35765   | PASS             |