
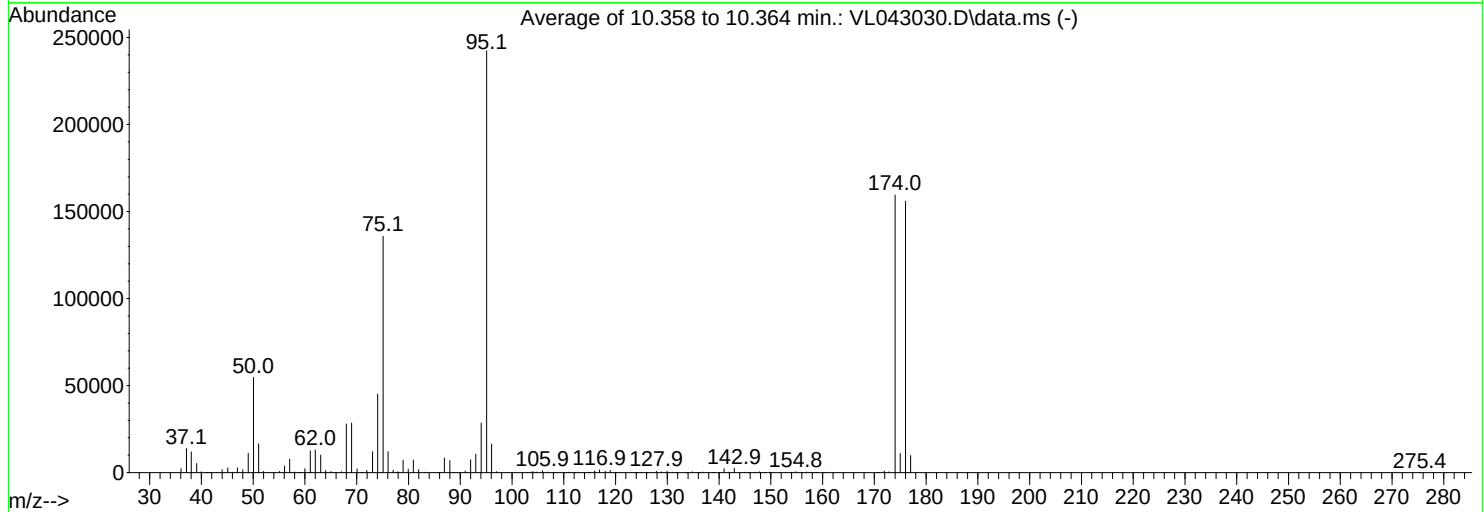


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100225\
Data File : VL043030.D
Acq On : 02 Oct 2025 09:11
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Oct 03 08:23:34 2025

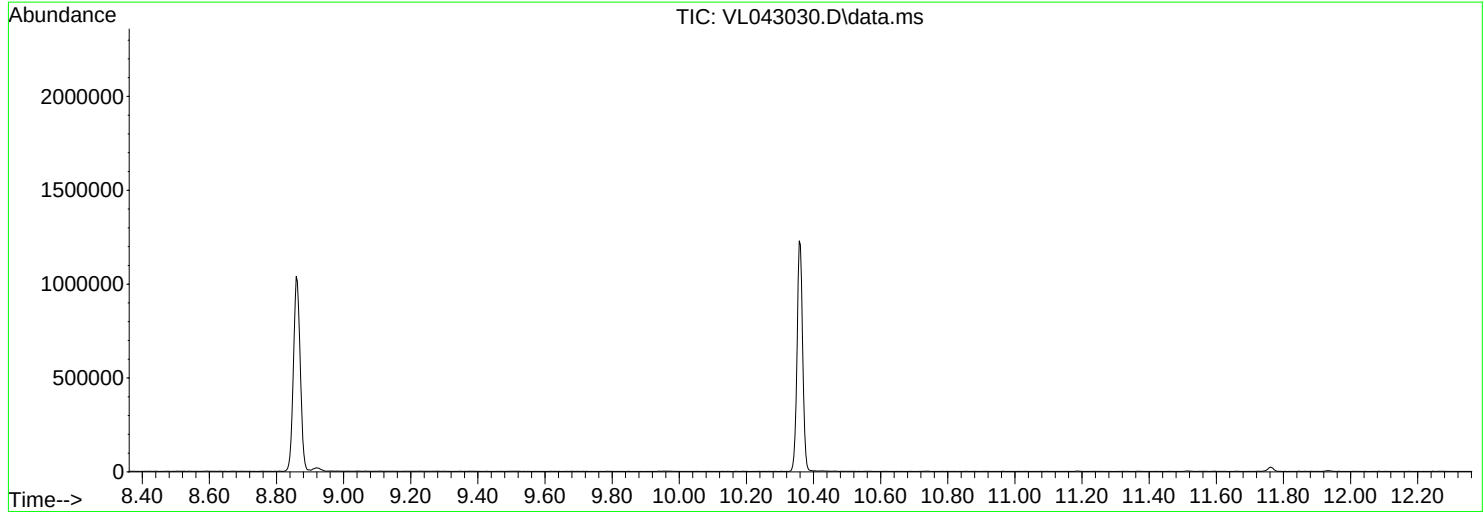

AutoFind: Scans 3173, 3174, 3175; Background Corrected with Scan 3150

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	22.6	54675	PASS
75	95	30	66	56.0	135808	PASS
95	95	100	100	100.0	242325	PASS
96	95	5	9	6.8	16496	PASS
173	174	0.00	2	0.3	425	PASS
174	95	50	120	65.8	159467	PASS
175	174	4	9	6.9	10992	PASS
176	174	93	101	97.8	156032	PASS
177	176	5	9	6.3	9819	PASS

Average of 10.358 to 10.364 min.: VL043030.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	2330	46.00	250	57.05	7765	68.00	2792
37.10	13813	46.95	2788	58.05	341	69.00	2847
38.05	11973	48.00	1655	58.90	23	70.05	217
39.10	5249	49.05	11158	60.00	2342	70.90	4
39.95	499	50.05	54675	61.05	12524	71.95	1265
40.85	55	51.05	16585	62.00	13090	73.05	12010
41.20	34	52.00	716	63.05	10089	74.05	45096
41.70	41	52.90	129	64.00	1213	75.10	135808
42.95	81	54.05	98	65.05	689	76.05	12035
44.00	1684	55.10	722	66.00	121	77.05	1348
45.10	2730	56.05	3773	67.05	550	77.80	302

Average of 10.358 to 10.364 min.: VL043030.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.95	470	90.95	1003	105.90	1116	115.05	175
78.95	7200	92.00	7351	106.90	274	115.95	1031
79.95	2063	93.00	10598	108.20	33	116.90	1577
80.95	7288	94.05	28587	109.80	55	118.00	866
81.95	1746	95.10	242325	110.10	57	118.95	1306
83.15	295	96.05	16496	110.60	86	119.90	24
85.80	79	97.00	519	110.90	247	123.15	68
86.10	77	103.00	84	111.80	125	123.80	49
86.95	8373	103.80	409	112.10	47	124.10	45
88.00	7029	104.05	570	112.85	231	125.00	87
88.70	108	104.80	377	114.80	216	125.90	51

Average of 10.358 to 10.364 min.: VL043030.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.10	36	136.85	338	146.10	106	156.85	394
126.90	57	138.80	48	146.90	145	157.80	61
127.90	861	139.90	127	147.80	477	158.70	92
128.85	474	140.10	57	148.00	163	158.90	179
129.95	745	140.95	2272	148.90	139	160.60	61
130.95	284	141.85	274	149.75	245	160.95	263
131.70	18	142.95	2445	151.85	217	170.55	65
133.70	47	144.00	140	152.90	112	170.95	95
133.90	37	144.90	270	153.85	189	171.90	906
134.85	499	145.75	191	154.85	593	172.80	425
136.10	34	145.90	163	156.10	138	174.00	159467

Average of 10.358 to 10.364 min.: VL043030.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.00	10992						
176.00	156032						
177.00	9819						
178.00	298						
275.40	22						

Instrument :

MSVOA_L

ClientSampleId :

BFB