
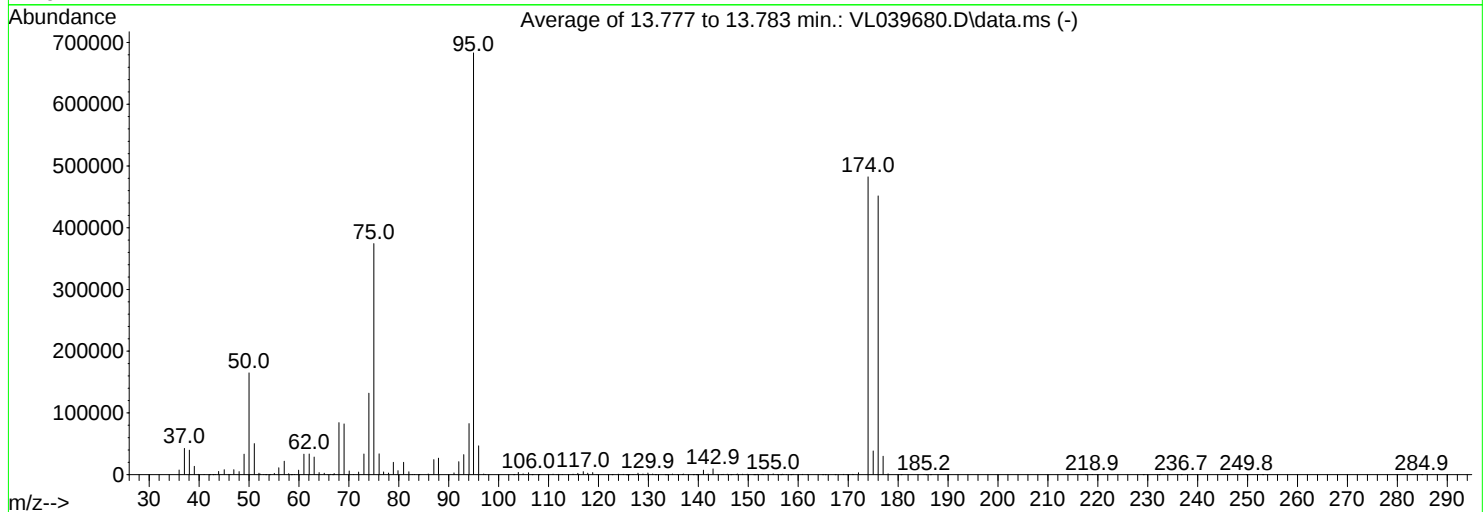


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100422\
Data File : VL039680.D
Acq On : 4 Oct 2022 12:32
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091922AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Mon Sep 19 14:26:28 2022

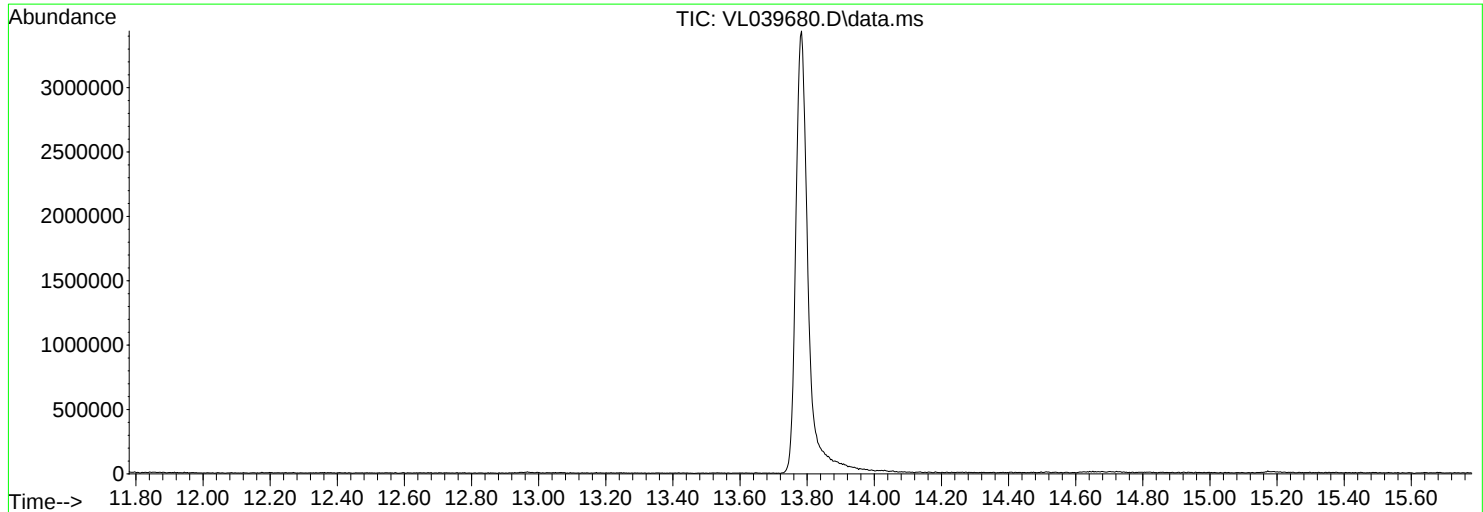

AutoFind: Scans 3475, 3476, 3477; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.1	164800	PASS
75	95	30	66	54.8	374272	PASS
95	95	100	100	100.0	683247	PASS
96	95	5	9	6.8	46739	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.6	482389	PASS
175	174	4	9	8.0	38456	PASS
176	174	93	101	93.6	451499	PASS
177	176	5	9	6.6	29715	PASS

Average of 13.777 to 13.783 min.: VL039680.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	7584	45.95	469	54.10	145	64.05	326
37.05	42643	46.20	178	55.05	2101	65.05	225
38.05	39784	46.95	7957	55.95	11058	65.80	30
39.05	13613	48.00	4993	57.05	21664	66.25	47
39.85	437	49.00	33099	57.95	1553	66.75	124
41.00	390	50.00	164800	58.50	91	67.05	1861
42.10	158	51.05	50291	59.10	405	68.00	84261
42.80	62	52.00	2314	59.95	7295	69.05	82120
43.25	367	52.20	1055	61.00	33104	70.05	5939
43.90	5170	52.95	199	62.05	33571	70.95	313
45.05	8020	53.35	125	63.05	28480	71.95	4125

Average of 13.777 to 13.783 min.: VL039680.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.00	33427	83.15	408	97.00	1124	111.70	215
74.00	131971	84.00	92	97.30	178	112.05	551
75.00	374272	85.90	1115	103.00	119	112.75	381
76.05	33611	87.00	24323	103.95	3594	113.95	171
76.95	4400	87.95	26811	104.90	1392	114.90	904
77.95	2644	91.05	2976	106.00	3115	115.85	2192
78.90	20029	92.00	21104	106.70	148	116.10	463
79.85	6402	93.00	32507	106.85	381	116.95	4934
80.95	19915	94.05	82563	108.05	152	117.85	2261
82.00	4546	94.95	683247	109.90	662	118.85	3476
82.70	169	96.00	46739	110.90	786	119.70	265

Average of 13.777 to 13.783 min.: VL039680.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
121.90	288	129.90	2534	139.80	166	147.60	525
122.70	69	130.85	1167	141.00	7385	147.85	1128
122.85	305	131.40	76	141.70	239	148.85	826
123.95	791	133.40	63	141.95	964	149.80	672
124.95	622	133.70	66	142.95	9235	151.10	133
125.60	83	134.80	1013	143.90	532	151.40	73
125.80	143	135.85	254	144.70	244	151.85	519
126.00	109	136.80	477	144.95	547	152.75	422
126.90	227	137.00	1134	145.80	743	153.00	246
127.90	2279	139.00	59	146.50	146	153.85	236
128.90	996	139.60	157	146.95	335	155.00	1388

Average of 13.777 to 13.783 min.: VL039680.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.85	334	167.40	62	178.00	1302	253.00	62
156.50	63	169.10	521	180.60	70	284.90	67
156.80	848	169.80	189	185.20	312		
157.10	209	170.15	334	185.60	63		
157.65	378	170.90	526	186.50	53		
158.50	146	171.10	310	217.60	84		
158.95	634	172.05	3022	218.90	234		
160.85	609	174.00	482389	229.10	65		
161.85	205	175.00	38456	232.30	50		
164.90	70	176.00	451499	236.70	67		
165.40	72	177.00	29715	249.80	72		