

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100423\
 Data File : VL040743.D
 Acq On : 4 Oct 2023 16:54
 Operator : SY/MD
 Sample : 04716-03DUP
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :

Quant Time: Oct 05 04:27:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091423AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Sep 19 05:12:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.192	49	955034	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.648	114	2675255	10.000	ppbv	-0.01
55) Chlorobenzene-d5	11.449	117	2269128	10.000	ppbv	-0.03
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.757	95	1724223	9.835	ppbv	-0.03
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.300%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.745	85	108482	0.516	ppbv	99
3) Chlorodifluoromethane	2.694	51	243122	1.563	ppbv #	78
9) Propene	2.886	41	303882	6.780	ppbv	96
10) Heptane	7.581	43	10876	0.108	ppbv #	26
11) Trichlorofluoromethane	3.575	101	44335	0.240	ppbv	96
12) 1,1,2-Trichlorotrifluo...	4.066	101	5058	0.038	ppbv #	7
13) Ethanol	3.250	45	361731	27.266	ppbv	98
15) Acetone	3.478	43	1887155	14.981	ppbv #	88
16) 1,3-Butadiene	2.980	39	19647	0.358	ppbv #	71
19) Isopropyl Alcohol	3.587	45	313133	4.125	ppbv #	88
20) Methylene Chloride	3.941	84	502904	7.417	ppbv	96
21) Allyl Chloride	3.964	41	8591	0.111	ppbv #	1
23) Vinyl Acetate	4.616	43	53467	0.410	ppbv #	1
25) Ethyl Acetate	5.211	43	286850	1.412	ppbv #	84
26) Hexane	5.214	57	361351	3.761	ppbv #	44
27) Carbon Disulfide	4.128	76	4797	0.036	ppbv #	1
30) Cyclohexane	6.607	84	4699	0.065	ppbv #	1
34) 2-Butanone	4.796	43	78046	0.580	ppbv	97
35) Carbon Tetrachloride	6.484	117	6817	0.037	ppbv	87
36) Benzene	6.369	78	111011	0.560	ppbv	94
38) Trichloroethene	7.285	130	2423	0.032	ppbv #	58
39) 1,2-Dichloropropane	6.648	63	625924	8.208	ppbv #	23
44) 2,2,4-Trimethylpentane	7.324	57	60796	0.193	ppbv #	26
50) 4-Methyl-2-Pentanone	8.185	43	6091	0.034	ppbv #	57
52) Tetrachloroethene	10.603	164	5033	0.078	ppbv #	82
53) Toluene	9.208	91	2660771	12.722	ppbv	99
58) Ethyl Benzene	12.076	91	59039	0.228	ppbv	91
59) m/p-Xylene	12.330	91	333026	1.371	ppbv	96
60) o-Xylene	13.040	91	117781	0.508	ppbv	98
61) Styrene	12.880	104	14626	0.151	ppbv #	42
72) 4-Ethyltoluene	15.179	105	76319	0.294	ppbv #	89
73) 1,3,5-Trimethylbenzene	15.339	105	80735	0.345	ppbv	91
74) 1,2,4-Trimethylbenzene	16.089	105	269088	0.944	ppbv #	68
80) Naphthalene,2-methyl-	24.368	142	1684	0.039	ppbv #	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_L

ClientSampleId :


Quant Time: Oct 05 04:27:49 2023


Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091423AIR.M

Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LFri Aug 26 06:05:16 2022

QLast Update : Tue Sep 19 05:12:43 2023


Response via : Initial Calibration

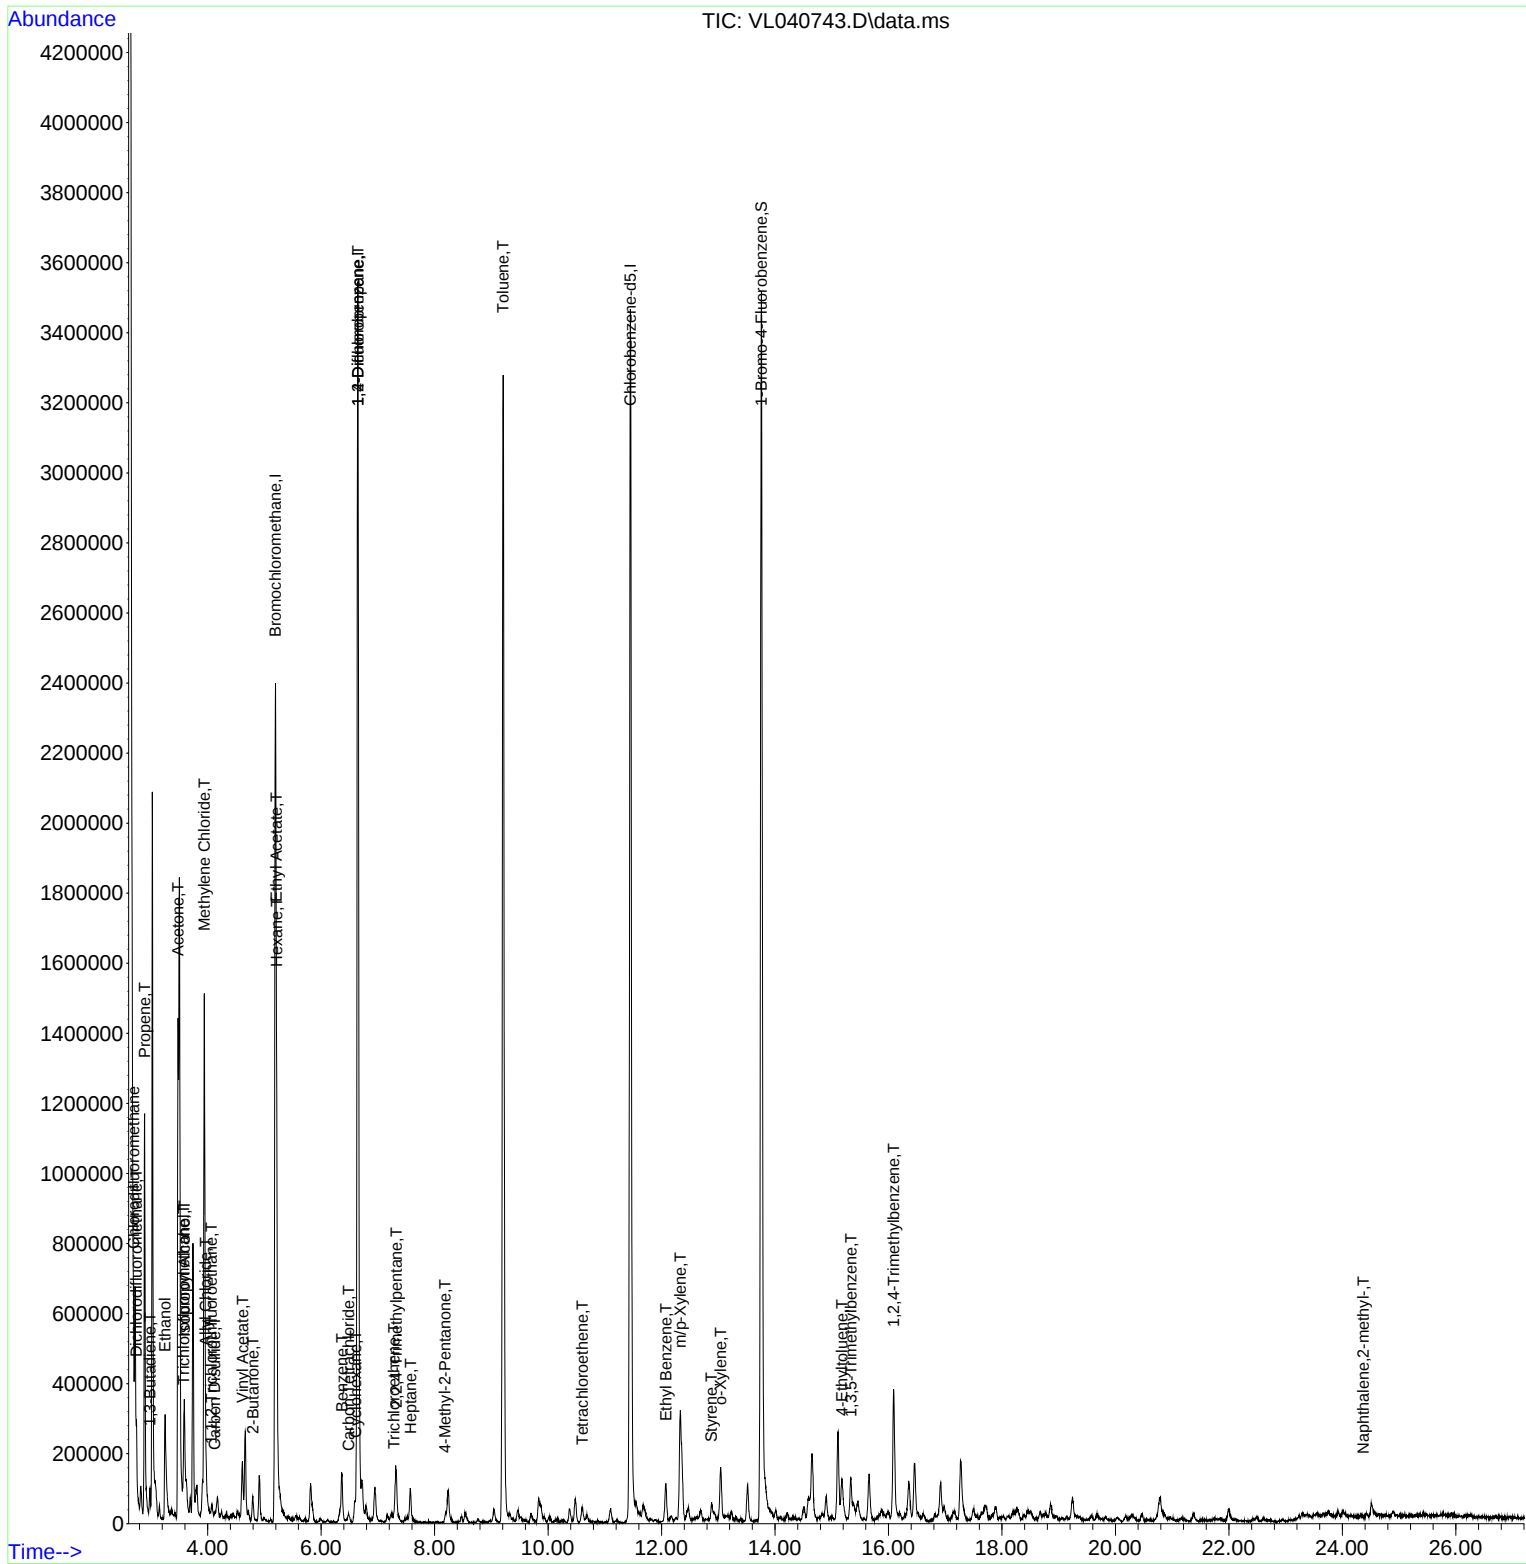






#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.192 min Scan# 80
Delta R.T. -0.006 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54


Instrument :
MSVOA_L
ClientSampleId :

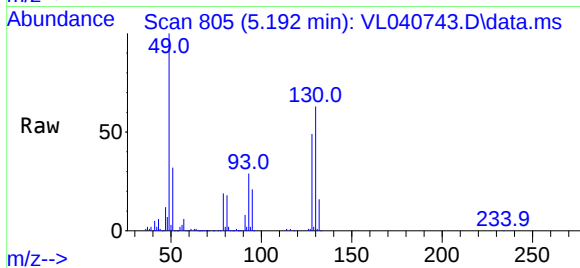



Tgt Ion: 49 Resp: 955034
Ion Ratio Lower Upper
49 100
128 54.0 25.4 76.0
130 68.6 32.3 96.8

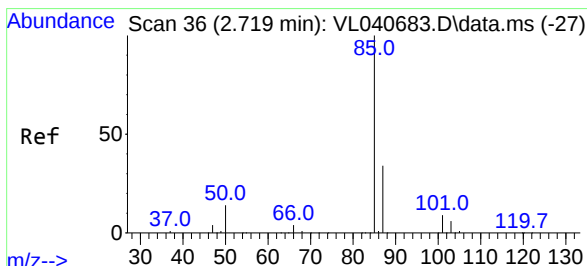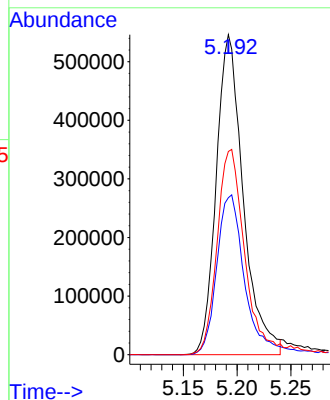


#2
Dichlorodifluoromethane
Concen: 0.516 ppbv
RT: 2.745 min Scan# 44
Delta R.T. 0.013 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

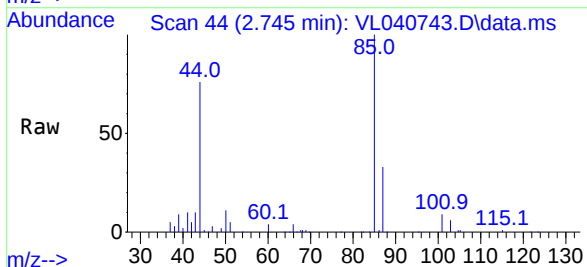

Tgt Ion: 85 Resp: 108482
Ion Ratio Lower Upper
85 100
87 33.6 27.2 40.8



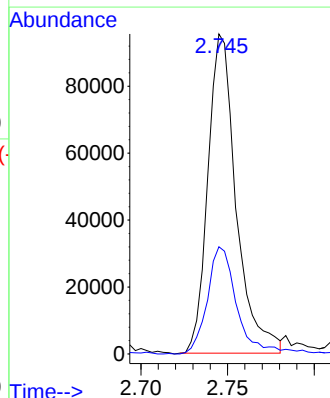
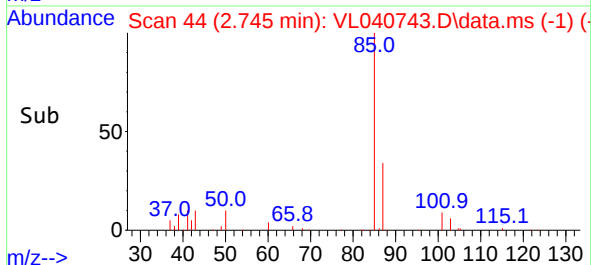


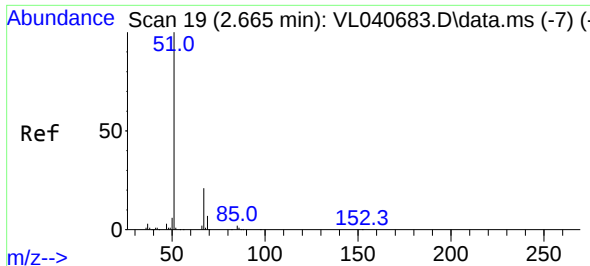

#3
Chlorodifluoromethane
Concen: 1.563 ppbv
RT: 2.694 min Scan# 21
Delta R.T. 0.016 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 51 Resp: 243122
Ion Ratio Lower Upper
51 100
67 10.8 16.7 25.1#

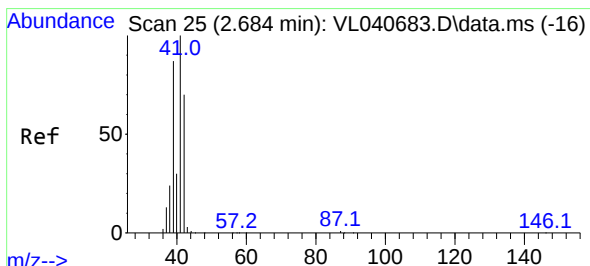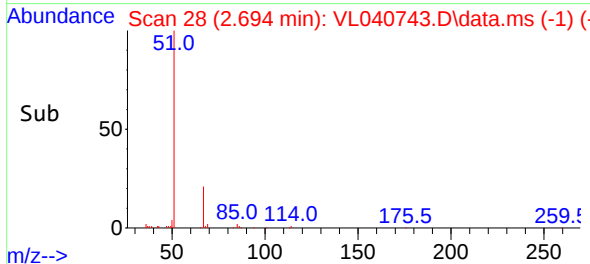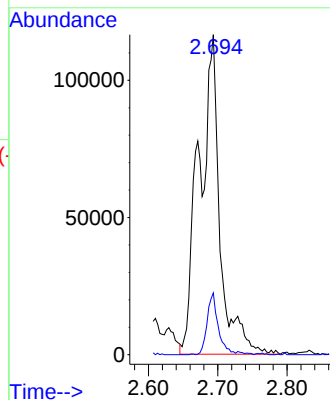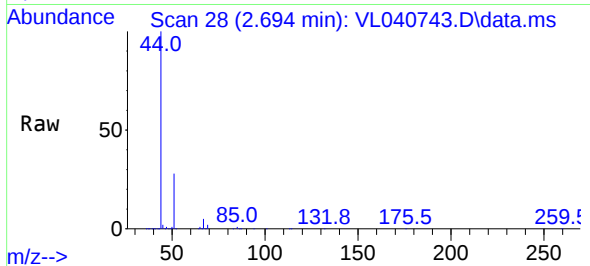

#9
Propene
Concen: 6.780 ppbv
RT: 2.886 min Scan# 88
Delta R.T. 0.190 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

Tgt Ion: 41 Resp: 303882
Ion Ratio Lower Upper
41 100
42 67.5 56.7 85.1

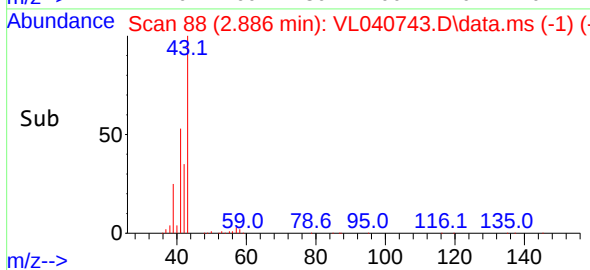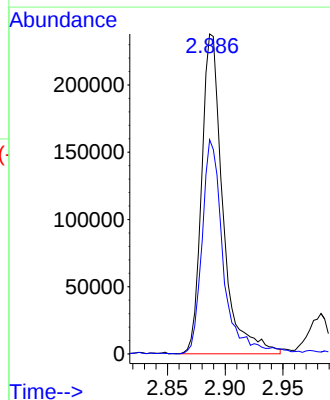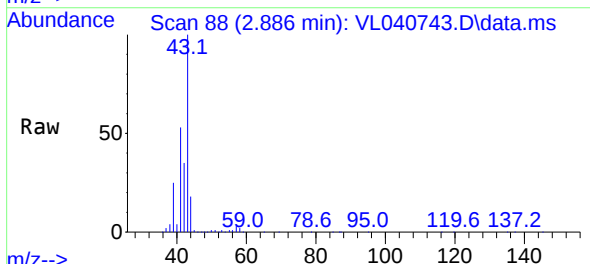



#10

Heptane

Concen: 0.108 ppbv

RT: 7.581 min Scan# 1

Delta R.T. -0.006 min

Lab File: VL040743.D

Acq: 4 Oct 2023 16:54

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion: 43 Resp: 10876

Ion Ratio Lower Upper

43 100

57 0.0 41.8 62.6#

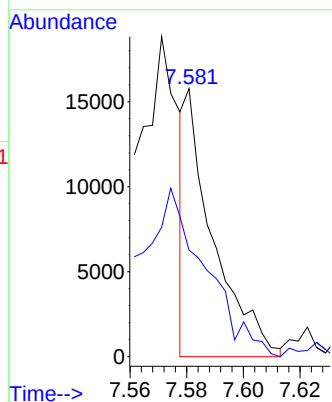

#11

Trichlorofluoromethane

Concen: 0.240 ppbv

RT: 3.575 min Scan# 302

Delta R.T. 0.007 min

Lab File: VL040743.D




Acq: 4 Oct 2023 16:54


Tgt Ion:101 Resp: 44335

Ion Ratio Lower Upper

101 100

103 61.3 51.3 76.9


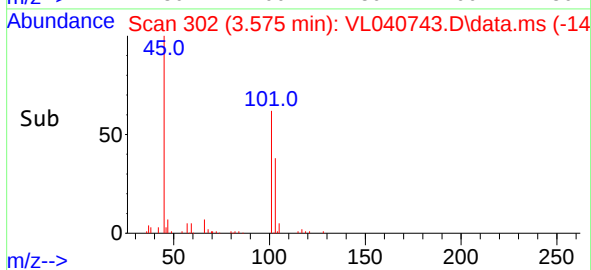






#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 0.038 ppbv
 RT: 4.066 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: VL040743.D
 Acq: 4 Oct 2023 16:54




Instrument :
 MSVOA_L
 ClientSampleId :


Tgt Ion:101 Resp: 5058
 Ion Ratio Lower Upper
 101 100
 151 147.8 56.8 85.2#

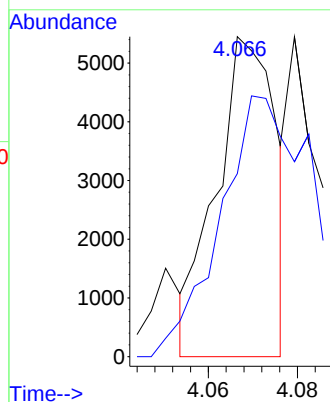

#13
 Ethanol
 Concen: 27.266 ppbv
 RT: 3.250 min Scan# 201
 Delta R.T. 0.007 min
 Lab File: VL040743.D
 Acq: 4 Oct 2023 16:54

Tgt Ion: 45 Resp: 361731
 Ion Ratio Lower Upper
 45 100
 46 37.1 15.2 61.0



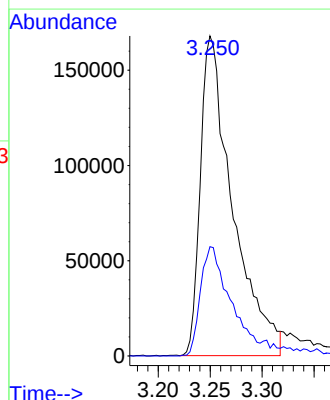





#15
Acetone
Concen: 14.981 ppbv
RT: 3.478 min Scan# 21
Delta R.T. 0.007 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 43 Resp: 1887155
Ion Ratio Lower Upper
43 100
58 22.0 22.6 34.0#

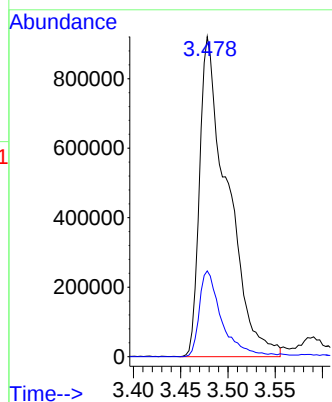

#16
1,3-Butadiene
Concen: 0.358 ppbv
RT: 2.980 min Scan# 117
Delta R.T. -0.010 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

Tgt Ion: 39 Resp: 19647
Ion Ratio Lower Upper
39 100
54 55.1 64.8 97.2#

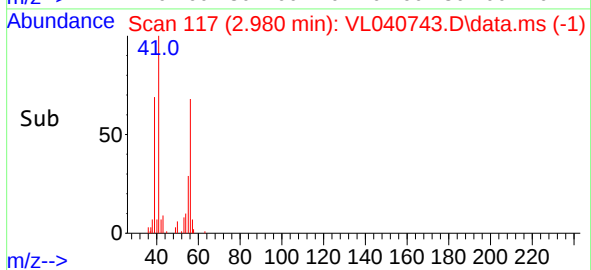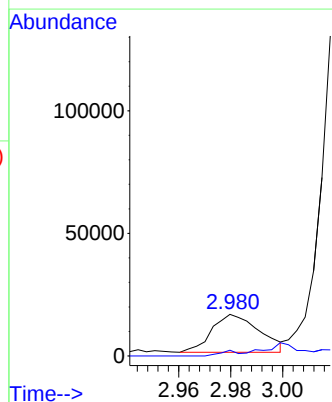



#19

Isopropyl Alcohol

Concen: 4.125 ppbv

RT: 3.587 min Scan# 306

Delta R.T. 0.010 min

Lab File: VL040743.D

Acq: 4 Oct 2023 16:54

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion: 45 Resp: 313133

Ion Ratio Lower Upper

45 100

58 6.4 1.9 2.9#

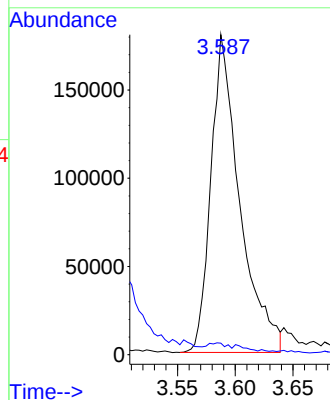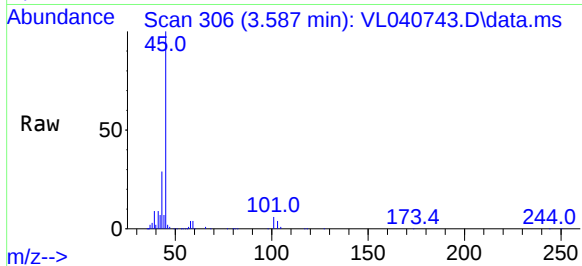

#20

Methylene Chloride

Concen: 7.417 ppbv

RT: 3.941 min Scan# 416

Delta R.T. 0.003 min

Lab File: VL040743.D

Acq: 4 Oct 2023 16:54

Tgt Ion: 84 Resp: 502904




Ion Ratio Lower Upper


84 100

49 148.6 114.4 171.6

51 46.5 35.5 53.3

86 63.1 53.2 79.8



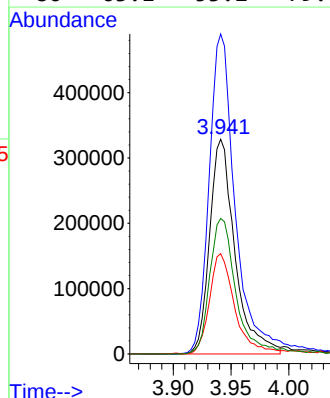
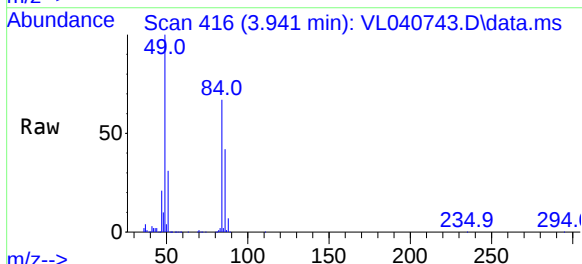




#21
Allyl Chloride
Concen: 0.111 ppbv
RT: 3.964 min Scan# 41
Delta R.T. -0.038 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 41 Resp: 8591
Ion Ratio Lower Upper
41 100
76 0.0 26.6 40.0#
39 199.4 65.0 97.4#



#23
Vinyl Acetate
Concen: 0.410 ppbv
RT: 4.616 min Scan# 626
Delta R.T. -0.016 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54


Tgt Ion: 43 Resp: 53467
Ion Ratio Lower Upper
43 100
86 11.4 5.6 8.4#
42 96.0 7.6 11.4#
44 4.1 5.0 7.4#

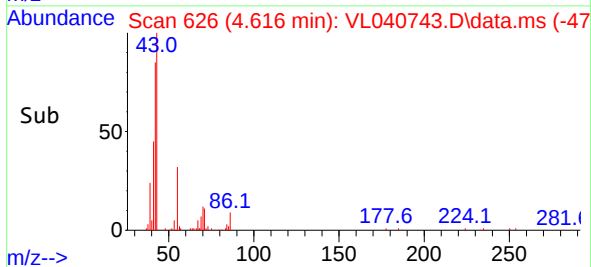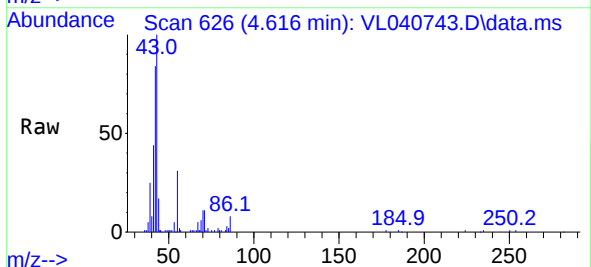






#25
Ethyl Acetate
Concen: 1.412 ppbv
RT: 5.211 min Scan# 811
Delta R.T. 0.000 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

Instrument :
MSVOA_L
ClientSampleId :







Tgt Ion: 43 Resp: 286850
Ion Ratio Lower Upper
43 100
45 4.4 8.2 12.4#
61 2.8 8.2 12.4#
70 3.2 5.9 8.9#

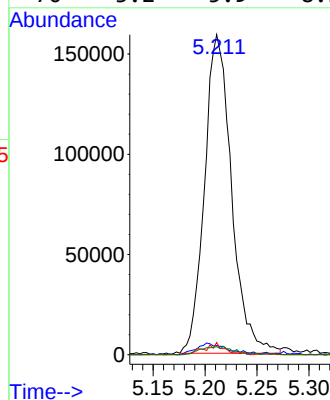

#26
Hexane
Concen: 3.761 ppbv
RT: 5.214 min Scan# 812
Delta R.T. -0.006 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

Tgt Ion: 57 Resp: 361351
Ion Ratio Lower Upper
57 100
41 90.6 75.2 112.8
43 82.5 185.6 278.4#
56 54.0 43.8 65.8



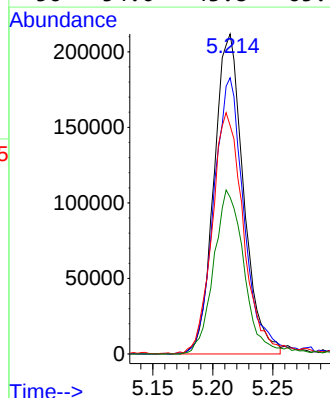





#27
Carbon Disulfide
Concen: 0.036 ppbv
RT: 4.128 min Scan# 41
Delta R.T. -0.003 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 76 Resp: 4797
Ion Ratio Lower Upper
76 100
44 157.0 14.5 21.7#
78 0.0 7.7 11.5#



#30
Cyclohexane
Concen: 0.065 ppbv
RT: 6.607 min Scan# 1245
Delta R.T. -0.003 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

Tgt Ion: 84 Resp: 4699
Ion Ratio Lower Upper
84 100
56 0.0 103.2 154.8#
41 0.0 65.5 98.3#

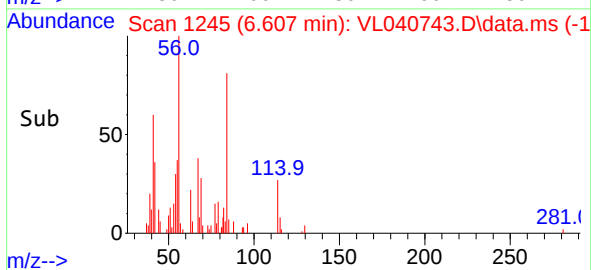



#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 6.648 min Scan# 11

Delta R.T. -0.013 min

Lab File: VL040743.D

Acq: 4 Oct 2023 16:54

Instrument :

MSVOA_L

ClientSampleId :





Tgt Ion:114 Resp: 2675255

Ion Ratio Lower Upper

114 100

63 24.1 21.1 31.7

88 17.5 14.5 21.7

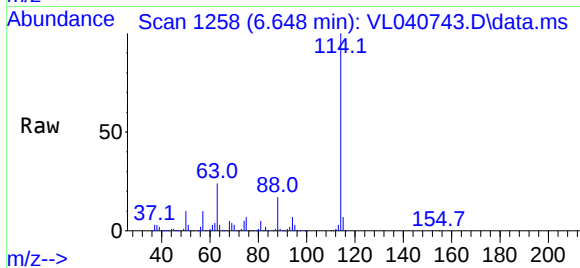

#34

2-Butanone

Concen: 0.580 ppbv

RT: 4.796 min Scan# 682

Delta R.T. 0.007 min

Lab File: VL040743.D




Acq: 4 Oct 2023 16:54


Tgt Ion: 43 Resp: 78046

Ion Ratio Lower Upper

43 100

72 24.6 18.6 27.8


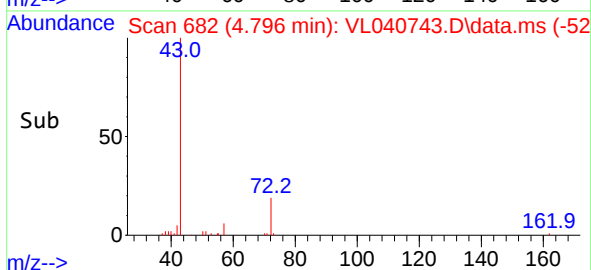
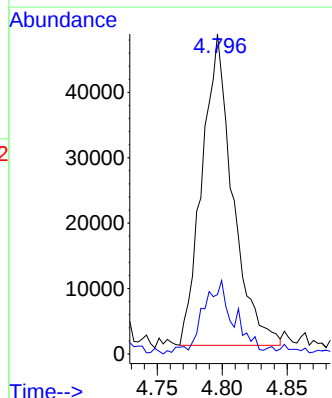
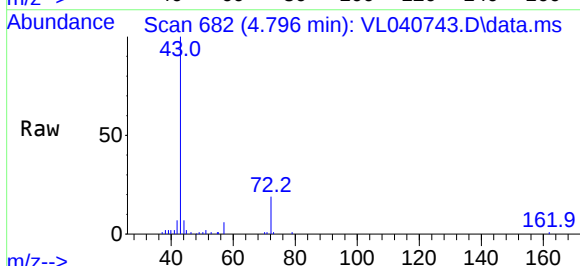




#35
Carbon Tetrachloride
Concen: 0.037 ppbv
RT: 6.484 min Scan# 1170
Delta R.T. -0.019 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion:117 Resp: 6817
Ion Ratio Lower Upper
117 100
119 81.3 78.6 117.8
121 31.8 24.7 37.1



#36
Benzene
Concen: 0.560 ppbv
RT: 6.369 min Scan# 1171
Delta R.T. -0.013 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54


Tgt Ion: 78 Resp: 111011
Ion Ratio Lower Upper
78 100
77 19.9 17.9 26.9
50 18.4 17.3 25.9

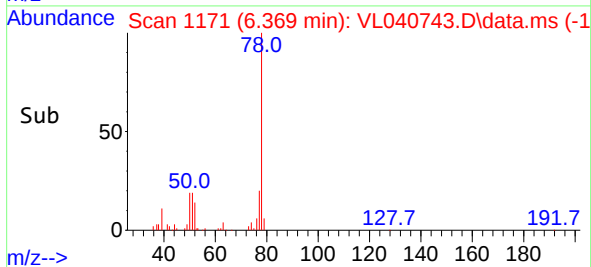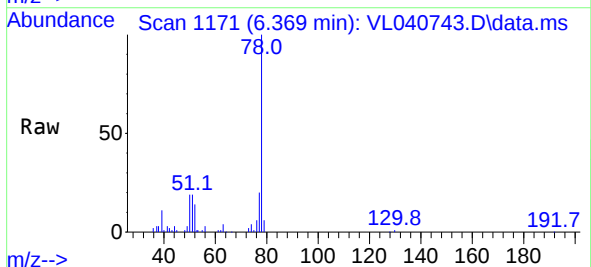






#38
 Trichloroethene
 Concen: 0.032 ppbv
 RT: 7.285 min Scan# 1456
 Delta R.T. -0.016 min
 Lab File: VL040743.D
 Acq: 4 Oct 2023 16:54

Instrument :
 MSVOA_L
 ClientSampleId :



Tgt Ion:130 Resp: 2423




Ion	Ratio	Lower	Upper
130	100		
95	130.7	91.9	137.9
132	40.7	77.3	115.9#
97	132.3	62.3	93.5#




#39
 1,2-Dichloropropane
 Concen: 8.208 ppbv
 RT: 6.648 min Scan# 1258
 Delta R.T. -0.434 min
 Lab File: VL040743.D
 Acq: 4 Oct 2023 16:54

Tgt Ion: 63 Resp: 625924

Ion	Ratio	Lower	Upper
63	100		
41	0.0	61.6	92.4#
62	17.0	55.8	83.8#


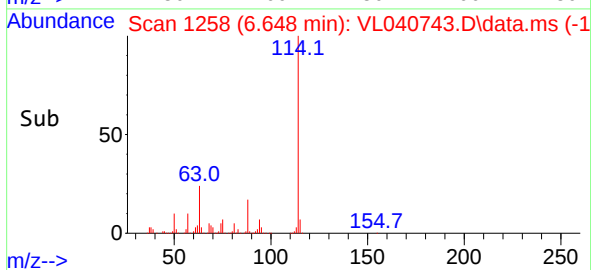






#44
2,2,4-Trimethylpentane
Concen: 0.193 ppbv
RT: 7.324 min Scan# 1467
Delta R.T. -0.013 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 57 Resp: 60796
Ion Ratio Lower Upper
57 100
41 0.0 28.5 42.7#
56 81.3 25.4 38.2#



#50
4-Methyl-2-Pentanone
Concen: 0.034 ppbv
RT: 8.185 min Scan# 1736
Delta R.T. -0.006 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54


Tgt Ion: 43 Resp: 6091
Ion Ratio Lower Upper
43 100
58 60.3 28.2 42.4#

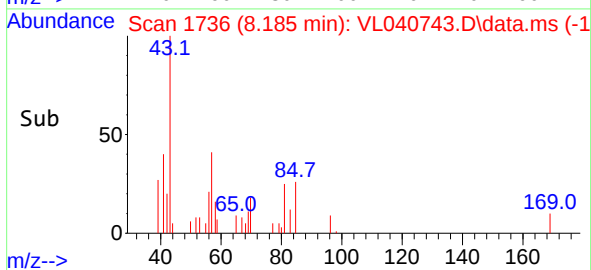






#52
Tetrachloroethene
Concen: 0.078 ppbv
RT: 10.603 min Scan# 2490
Delta R.T. -0.022 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

Instrument :
MSVOA_L
ClientSampleId :

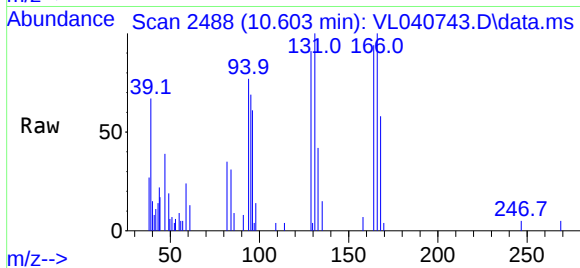

Tgt Ion:164 Resp: 5033




Ion	Ratio	Lower	Upper
164	100		
166	84.0	103.4	155.2#
129	95.2	83.5	125.3
131	104.8	83.4	125.0

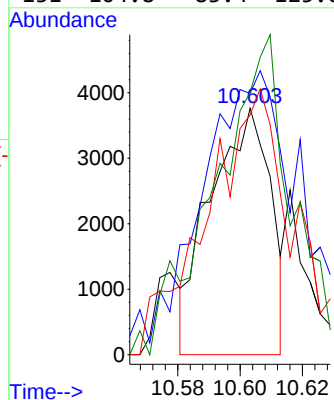


#53
Toluene
Concen: 12.722 ppbv
RT: 9.208 min Scan# 2054
Delta R.T. -0.022 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

Tgt Ion: 91 Resp: 2660771

Ion	Ratio	Lower	Upper
91	100		
92	61.6	48.5	72.7


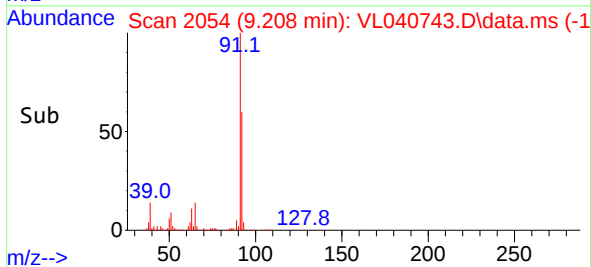
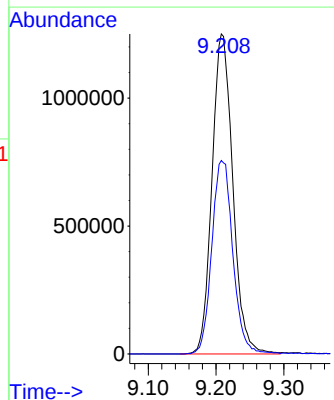
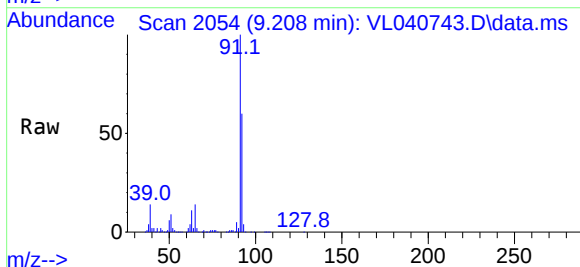




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.449 min Scan# 21
Delta R.T. -0.029 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion:117 Resp: 2269128
Ion Ratio Lower Upper
117 100
82 63.5 51.4 77.0
119 32.3 24.7 37.1

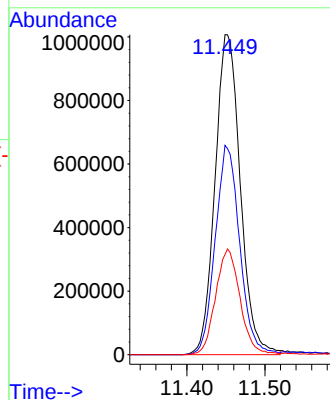

#58
Ethyl Benzene
Concen: 0.228 ppbv
RT: 12.076 min Scan# 2946
Delta R.T. -0.026 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

Tgt Ion: 91 Resp: 59039
Ion Ratio Lower Upper
91 100
106 36.1 24.7 37.1

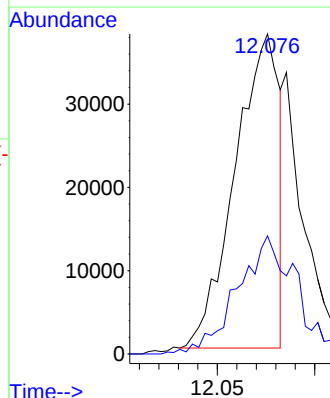



#59

m/p-Xylene

Concen: 1.371 ppbv

RT: 12.330 min Scan# 3037

Delta R.T. -0.051 min

Lab File: VL040743.D

Acq: 4 Oct 2023 16:54

Instrument :

MSVOA_L


ClientSampleId :

Tgt Ion: 91 Resp: 333026




Ion Ratio Lower Upper

91 100

106 45.9 34.8 52.2

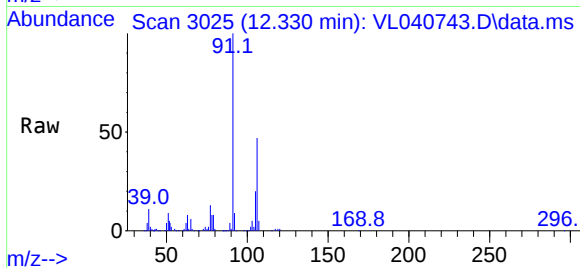

Abundance

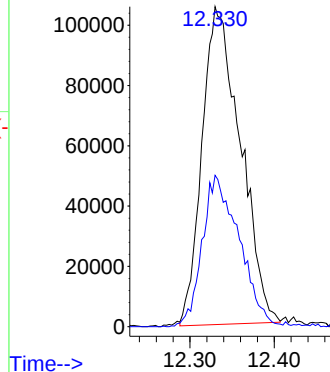

#60

o-Xylene

Concen: 0.508 ppbv

RT: 13.040 min Scan# 3246

Delta R.T. -0.029 min

Lab File: VL040743.D


Acq: 4 Oct 2023 16:54

Tgt Ion: 91 Resp: 117781



Ion Ratio Lower Upper


91 100

106 43.6 22.3 66.9

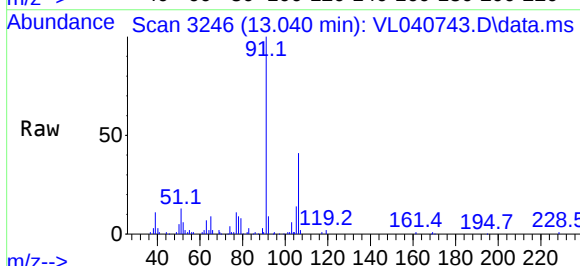

Abundance



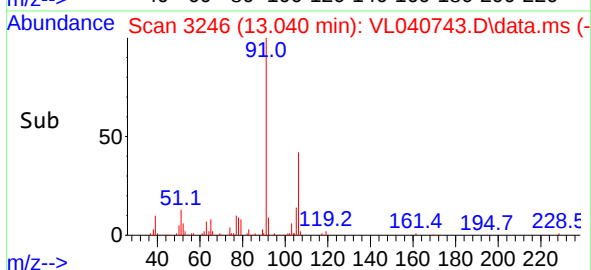
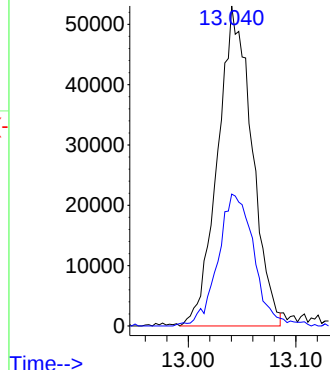




#61
Styrene
Concen: 0.151 ppbv
RT: 12.880 min Scan# 3196
Delta R.T. -0.026 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion:104 Resp: 14626
Ion Ratio Lower Upper
104 100
78 92.6 43.4 65.0#
103 88.7 37.2 55.8#

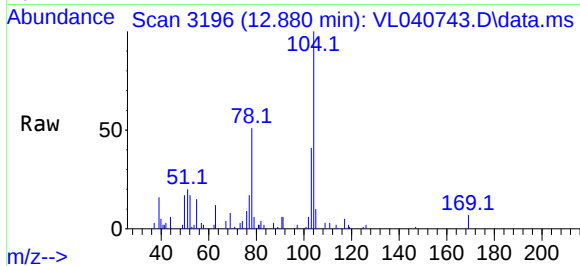

#68
1-Bromo-4-Fluorobenzene
Concen: 9.835 ppbv
RT: 13.757 min Scan# 3469
Delta R.T. -0.029 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54


Tgt Ion: 95 Resp: 1724223
Ion Ratio Lower Upper
95 100
174 62.3 48.9 73.3
175 4.5 3.5 5.3

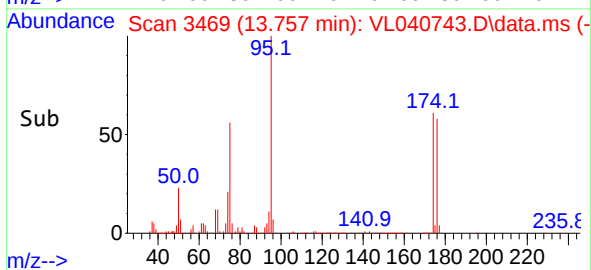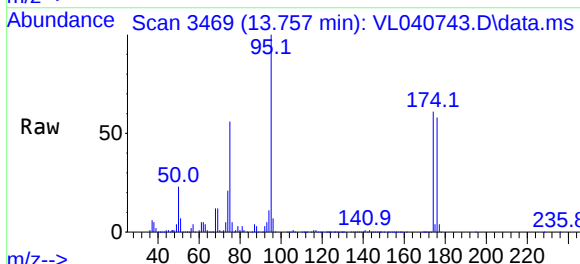






#72
4-Ethyltoluene
Concen: 0.294 ppbv
RT: 15.179 min Scan# 3911
Delta R.T. -0.022 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

Instrument :
MSVOA_L
ClientSampleId :







Tgt Ion:	105	Resp:	76319
Ion	Ratio	Lower	Upper
105	100		
120	33.0	23.9	35.9
91	22.3	11.0	16.4#
77	19.8	11.4	17.2#



#73
1,3,5-Trimethylbenzene
Concen: 0.345 ppbv
RT: 15.339 min Scan# 3961
Delta R.T. -0.022 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54


Tgt Ion:	105	Resp:	80735
Ion	Ratio	Lower	Upper
105	100		
120	39.1	36.1	54.1

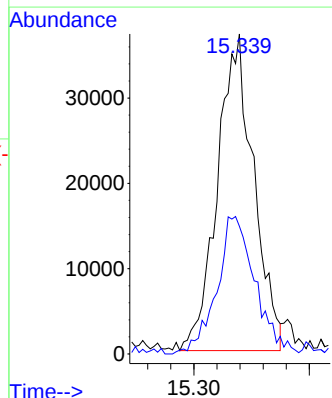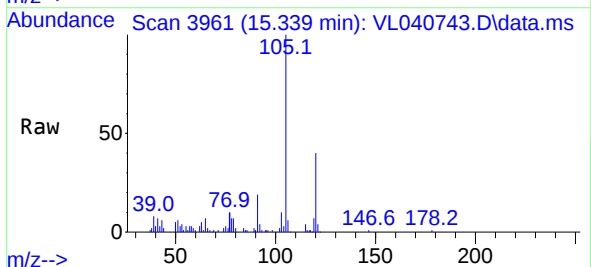






#74
1,2,4-Trimethylbenzene
Concen: 0.944 ppbv
RT: 16.089 min Scan# 4198
Delta R.T. -0.029 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

Instrument :
MSVOA_L
ClientSampleId :

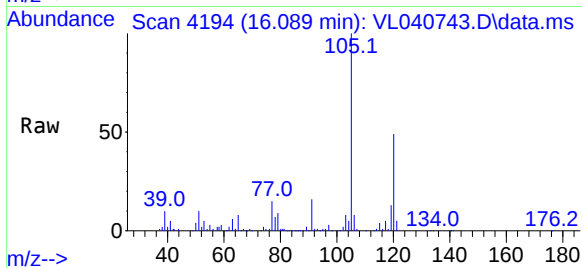

Tgt Ion:105 Resp: 269088
Ion Ratio Lower Upper
105 100
120 49.1 38.6 57.8
91 15.3 50.0 75.0#
77 14.9 20.6 31.0#



#80
Naphthalene,2-methyl-
Concen: 0.039 ppbv
RT: 24.368 min Scan# 6769
Delta R.T. -0.013 min
Lab File: VL040743.D
Acq: 4 Oct 2023 16:54

Tgt Ion:142 Resp: 1684
Ion Ratio Lower Upper
142 100
141 52.7 67.0 100.6#
115 37.4 37.4 56.2#

