
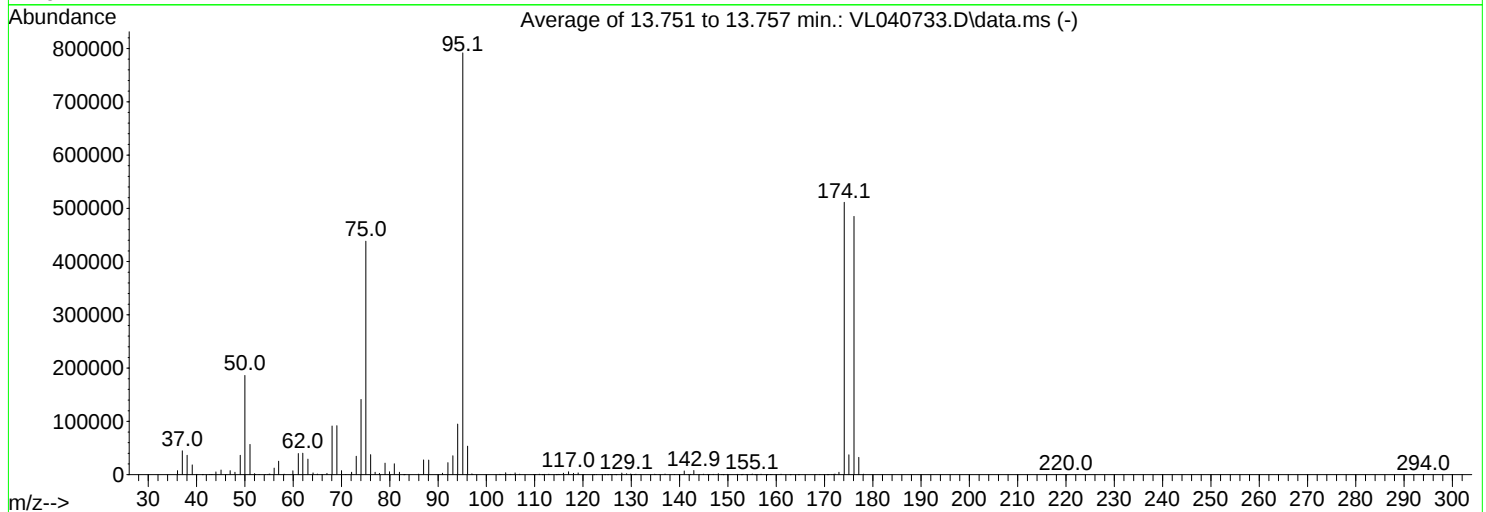


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100423\
 Data File : VL040733.D
 Acq On : 4 Oct 2023 9:22
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091423AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Sep 19 05:12:43 2023

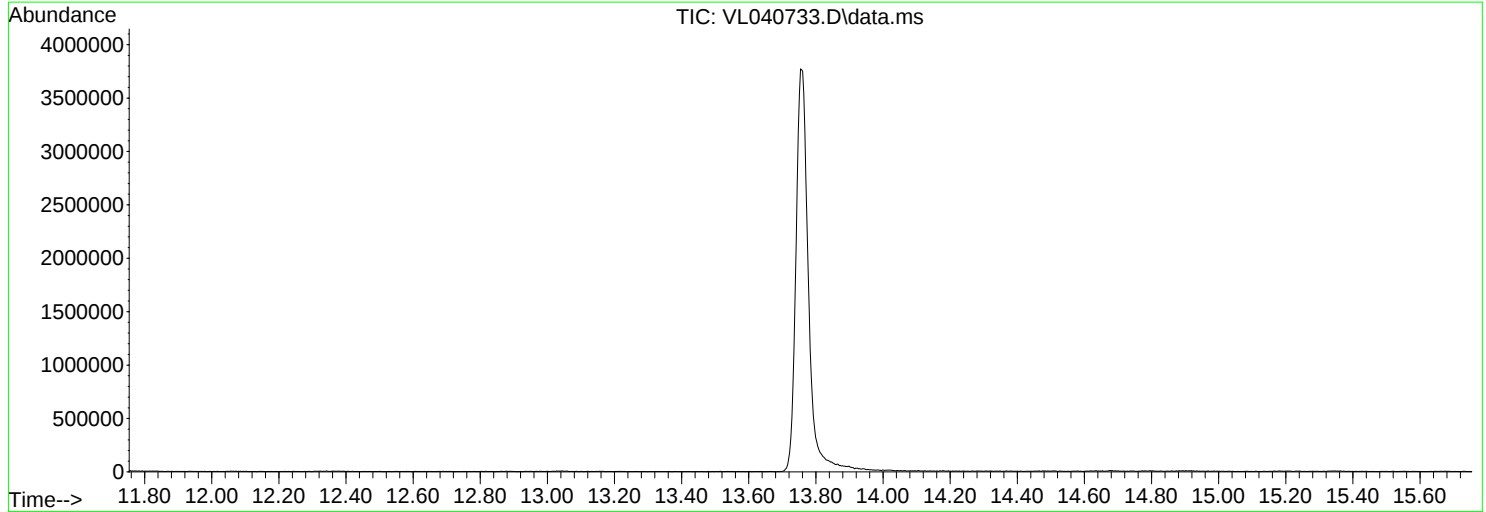

AutoFind: Scans 3467, 3468, 3469; Background Corrected with Scan 3444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.5	186283	PASS
75	95	30	66	55.3	438315	PASS
95	95	100	100	100.0	791915	PASS
96	95	5	9	6.8	53517	PASS
173	174	0.00	2	0.9	4646	PASS
174	95	50	120	64.5	511147	PASS
175	174	4	9	7.3	37293	PASS
176	174	93	101	94.9	484885	PASS
177	176	5	9	6.7	32539	PASS

Average of 13.751 to 13.757 min.: VL040733.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7630	46.05	369	55.00	789	65.95	191
37.05	44861	46.95	7427	55.15	1261	67.00	257
38.05	36413	47.95	4644	56.05	12295	68.05	9146
39.10	18293	49.05	36440	57.00	25299	69.05	9209
40.05	712	50.00	186283	58.10	1031	70.00	7580
41.20	93	51.05	56677	59.95	7185	70.90	379
42.70	210	52.00	1853	61.05	39571	72.10	4619
43.00	292	52.20	636	62.00	40389	73.05	34683
43.20	205	52.95	317	63.05	29227	74.05	141056
44.00	5060	54.20	179	64.10	3228	75.05	438315
45.05	8580	54.70	176	65.00	1283	76.05	37640

Average of 13.751 to 13.757 min.: VL040733.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.95	4454	90.90	2682	104.90	353	115.00	694
77.85	2304	92.05	22480	105.05	631	115.20	229
79.00	21533	93.05	35491	105.95	3228	115.95	2789
79.95	5531	94.05	95043	106.90	935	117.00	5495
80.95	20533	95.10	791915	109.80	247	118.05	2539
82.00	4462	96.10	53517	110.20	230	119.00	3246
82.90	61	97.00	1418	110.95	1072	120.00	81
83.15	422	97.20	299	111.60	67	122.20	112
85.95	872	102.75	615	112.05	571	122.80	177
87.00	27768	103.00	395	112.95	811	123.95	427
88.05	27323	104.00	3583	114.50	144	124.50	159

Average of 13.751 to 13.757 min.: VL040733.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.10	98	131.85	354	144.10	237	153.10	492
125.70	162	134.85	837	144.95	1044	153.80	300
126.00	311	135.10	276	145.85	518	154.10	275
126.60	316	135.75	164	146.20	435	154.80	308
126.80	55	137.00	1241	146.95	750	155.05	1301
128.05	2944	138.90	299	148.00	1739	155.60	120
129.05	1704	139.90	403	148.75	316	156.00	368
129.85	1276	140.95	7048	149.00	122	156.20	213
130.10	589	141.85	398	149.95	662	156.85	1047
130.70	208	142.25	685	151.95	643	158.10	74
130.95	940	142.95	7693	152.80	119	158.80	223

Average of 13.751 to 13.757 min.: VL040733.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
159.10	353	172.15	1101				
161.00	807	173.00	4646				
162.90	54	174.10	511147				
164.60	55	175.05	37293				
168.20	164	176.10	484885				
169.00	278	177.10	32539				
169.90	265	178.05	1059				
170.60	142	220.00	61				
170.95	257	294.00	84				
171.50	302						
171.90	526						