

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100521\
 Data File : VL037773.D
 Acq On : 5 Oct 2021 14:41
 Operator : SY/AP
 Sample : M4012-03
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 C0P17

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 3
 Start Thrs: 0.001
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.867	9	25	94	rBV	10440551	45766166	73.74%	16.238%
2	3.195	116	127	143	rBV	994400	1680034	2.71%	0.596%
3	3.597	236	252	274	rBV	325409	737138	1.19%	0.262%
4	3.835	318	326	348	rBV	1275343	2685928	4.33%	0.953%
5	3.960	352	365	393	rVV	2631499	6073413	9.79%	2.155%
6	4.333	470	481	505	rBV	1922748	3698206	5.96%	1.312%
7	5.655	879	892	907	rBV3	2651963	6447644	10.39%	2.288%
8	5.735	907	917	955	rVB	5393634	12032734	19.39%	4.269%
9	7.159	1343	1360	1378	rBV	4443157	9399663	15.15%	3.335%
10	11.204	2597	2618	2639	rBV3	9161106	22440007	36.16%	7.962%
11	11.670	2741	2763	2787	rBV2	2234537	6193761	9.98%	2.198%
12	12.063	2866	2885	2910	rBV	4472679	11077390	17.85%	3.930%
13	12.323	2953	2966	2982	rVB6	288331	708553	1.14%	0.251%
14	14.391	3591	3609	3659	rBV3	4132668	11871822	19.13%	4.212%
15	15.291	3879	3889	3905	rVB4	398636	994268	1.60%	0.353%
16	16.101	4118	4141	4158	rVB3	479668	1334989	2.15%	0.474%
17	16.960	4383	4408	4438	rBV2	19211209	62060841	100.00%	22.020%
18	17.088	4440	4448	4468	rVB6	389943	1192228	1.92%	0.423%
19	17.657	4614	4625	4643	rVB2	303964	822643	1.33%	0.292%
20	17.915	4684	4705	4739	rBV5	1915081	5738290	9.25%	2.036%
21	18.153	4760	4779	4795	rBV3	644263	1731220	2.79%	0.614%
22	18.333	4816	4835	4853	rBV2	4405836	12206914	19.67%	4.331%
23	18.394	4853	4854	4876	rVB5	472753	972590	1.57%	0.345%
24	18.786	4958	4976	4991	rVV3	495852	1588588	2.56%	0.564%
25	18.882	4991	5006	5020	rVV	3055128	8676663	13.98%	3.079%
26	18.931	5020	5021	5039	rVB2	914352	1531852	2.47%	0.544%
27	19.040	5039	5055	5070	rBV3	2007819	4974715	8.02%	1.765%
28	19.188	5084	5101	5116	rVB5	553270	1507427	2.43%	0.535%
29	19.435	5155	5178	5208	rVB5	1752187	5993336	9.66%	2.126%
30	21.451	5775	5805	5835	rBV2	7663583	28572625	46.04%	10.138%
31	22.773	6200	6216	6231	rVB5	435469	1130814	1.82%	0.401%


Sum of corrected areas: 281842462

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100521\
Data File : VL037773.D
Acq On : 5 Oct 2021 14:41
Operator : SY/AP
Sample : M4012-03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P17

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

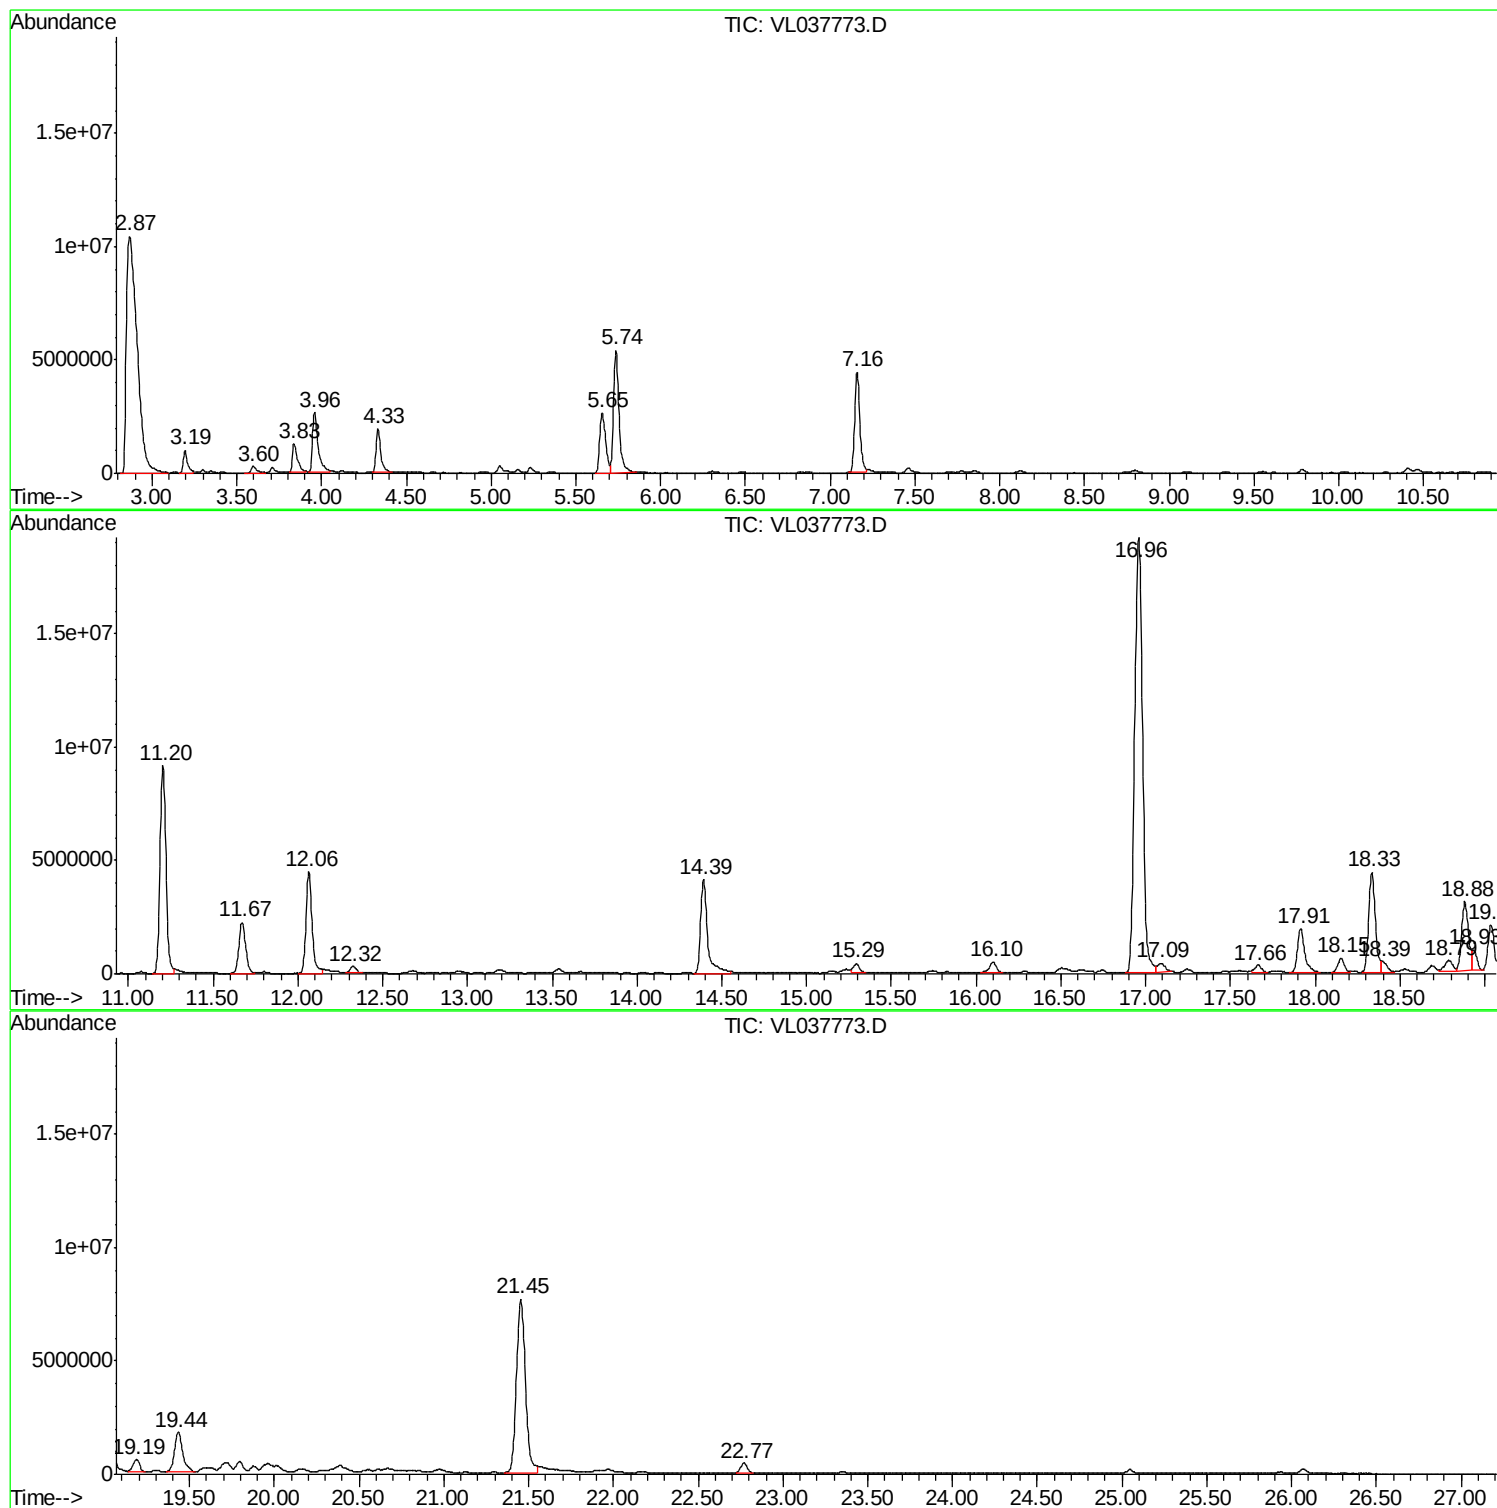

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100521\
Data File : VL037773.D
Acq On : 5 Oct 2021 14:41
Operator : SY/AP
Sample : M4012-03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P17

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100521\
Data File : VL037773.D
Acq On : 5 Oct 2021 14:41
Operator : SY/AP
Sample : M4012-03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P17

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc