

Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL100521\
 Data File : VL037781.D
 Acq On : 5 Oct 2021 19:59
 Operator : SY/AP
 Sample : M4012-10
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 C0P01

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 3
 Start Thrs: 0.001
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.864	6	24	88	rBV	11156216	52268508	100.00%	17.817%
2	3.189	116	125	142	rBV	772114	1344907	2.57%	0.458%
3	3.417	185	196	208	rBV	565117	928704	1.78%	0.317%
4	3.832	314	325	352	rBV	1045242	2677589	5.12%	0.913%
5	3.954	352	363	382	rVB	432772	952440	1.82%	0.325%
6	4.327	469	479	506	rBV	4545510	8769664	16.78%	2.989%
7	5.089	709	716	726	rVV3	297560	573677	1.10%	0.196%
8	5.147	726	734	750	rVV2	861760	1665518	3.19%	0.568%
9	5.652	875	891	910	rBV3	2812800	7757160	14.84%	2.644%
10	5.729	910	915	938	rVB3	280778	601822	1.15%	0.205%
11	6.298	1078	1092	1112	rBV3	332765	804618	1.54%	0.274%
12	7.153	1332	1358	1376	rBV	4144366	8982733	17.19%	3.062%
13	7.449	1436	1450	1480	rBV3	1476677	3677610	7.04%	1.254%
14	7.841	1561	1572	1590	rVB6	277615	681326	1.30%	0.232%
15	8.108	1640	1655	1670	rBV7	200288	531859	1.02%	0.181%
16	8.793	1858	1868	1879	rVB5	344827	772367	1.48%	0.263%
17	9.780	2164	2175	2188	rBV3	301810	639714	1.22%	0.218%
18	10.397	2351	2367	2378	rBV3	1288197	2945601	5.64%	1.004%
19	10.462	2380	2387	2398	rVB8	284202	627166	1.20%	0.214%
20	11.201	2595	2617	2640	rBV2	16268803	41209394	78.84%	14.047%
21	11.667	2737	2762	2784	rBV3	1918724	5195484	9.94%	1.771%
22	12.060	2867	2884	2909	rBV2	4209799	10389219	19.88%	3.541%
23	12.323	2948	2966	2984	rVB4	543865	1326765	2.54%	0.452%
24	12.941	3144	3158	3180	rBV4	258675	828798	1.59%	0.283%
25	13.529	3325	3341	3357	rBV4	602776	1541759	2.95%	0.526%
26	14.387	3591	3608	3627	rBV	3967042	10230499	19.57%	3.487%
27	15.223	3853	3868	3878	rVV9	190124	589781	1.13%	0.201%
28	16.098	4115	4140	4158	rBV2	657232	1983706	3.80%	0.676%
29	16.494	4248	4263	4278	rBV4	244293	734971	1.41%	0.251%
30	16.600	4280	4296	4314	rVV9	271677	840237	1.61%	0.286%
31	16.953	4382	4406	4440	rBV2	10428339	33149638	63.42%	11.300%
32	17.664	4608	4627	4641	rVB3	462829	1197747	2.29%	0.408%
33	17.908	4685	4703	4736	rBV2	1876849	5566981	10.65%	1.898%
34	18.146	4755	4777	4793	rBV3	743963	2076293	3.97%	0.708%

Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL100521\
Data File : VL037781.D
Acq On : 5 Oct 2021 19:59
Operator : SY/AP
Sample : M4012-10
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P01

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 3 Min Area: 3 % of largest Peak
Start Thrs: 0.001 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

35	18.333	4812	4835	4852	rBV3	6458052	18131742	34.69%	6.180%
36	18.397	4852	4855	4878	rVB2	627537	1369510	2.62%	0.467%
37	18.686	4929	4945	4958	rBV4	368471	1002782	1.92%	0.342%
38	18.783	4958	4975	4987	rVV6	592121	1920616	3.67%	0.655%
39	18.879	4987	5005	5017	rVV3	4527237	12847496	24.58%	4.379%
40	18.934	5017	5022	5037	rVB3	1359049	2849956	5.45%	0.971%
41	19.034	5037	5053	5069	rBV2	2473769	6188762	11.84%	2.110%
42	19.182	5080	5099	5115	rVB4	807179	2282710	4.37%	0.778%
43	19.429	5156	5176	5209	rBV6	2278769	8482767	16.23%	2.891%
44	19.709	5245	5263	5264	rBV3	367736	645519	1.24%	0.220%
45	19.722	5264	5267	5278	rVV3	394863	642552	1.23%	0.219%
46	19.792	5278	5289	5305	rVB5	530276	1311239	2.51%	0.447%
47	20.008	5350	5356	5383	rVB10	306473	983965	1.88%	0.335%
48	21.451	5779	5805	5831	rBV	5523638	19894173	38.06%	6.781%
49	22.763	6199	6213	6226	rBV4	308831	753087	1.44%	0.257%


Sum of corrected areas: 293371131

Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL100521\
Data File : VL037781.D
Acq On : 5 Oct 2021 19:59
Operator : SY/AP
Sample : M4012-10
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

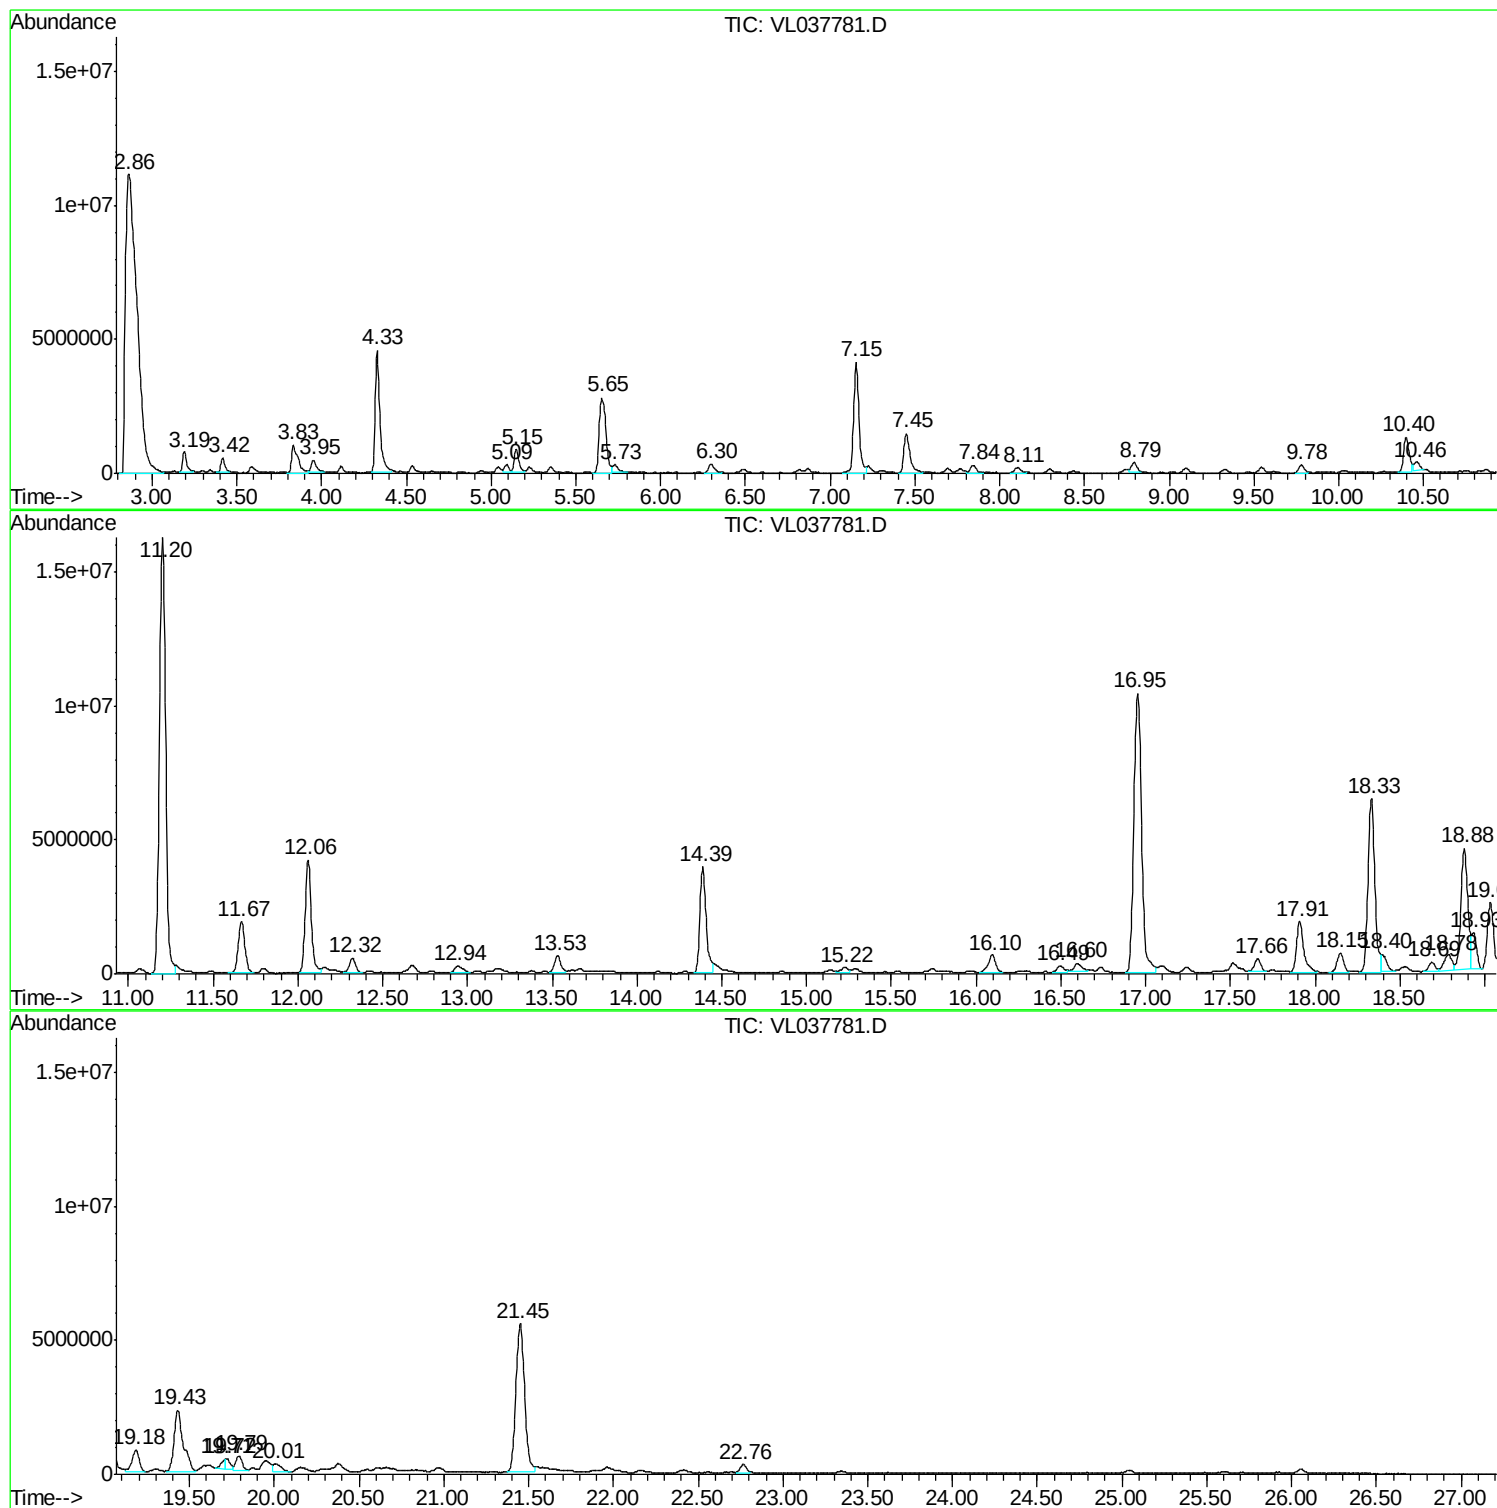

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100521\
Data File : VL037781.D
Acq On : 5 Oct 2021 19:59
Operator : SY/AP
Sample : M4012-10
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100521\
Data File : VL037781.D
Acq On : 5 Oct 2021 19:59
Operator : SY/AP
Sample : M4012-10
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc