


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL100521\
 Data File : VL037766.D
 Acq On : 5 Oct 2021 7:48
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021
 Last Update : Mon Oct 04 17:43:54 2021

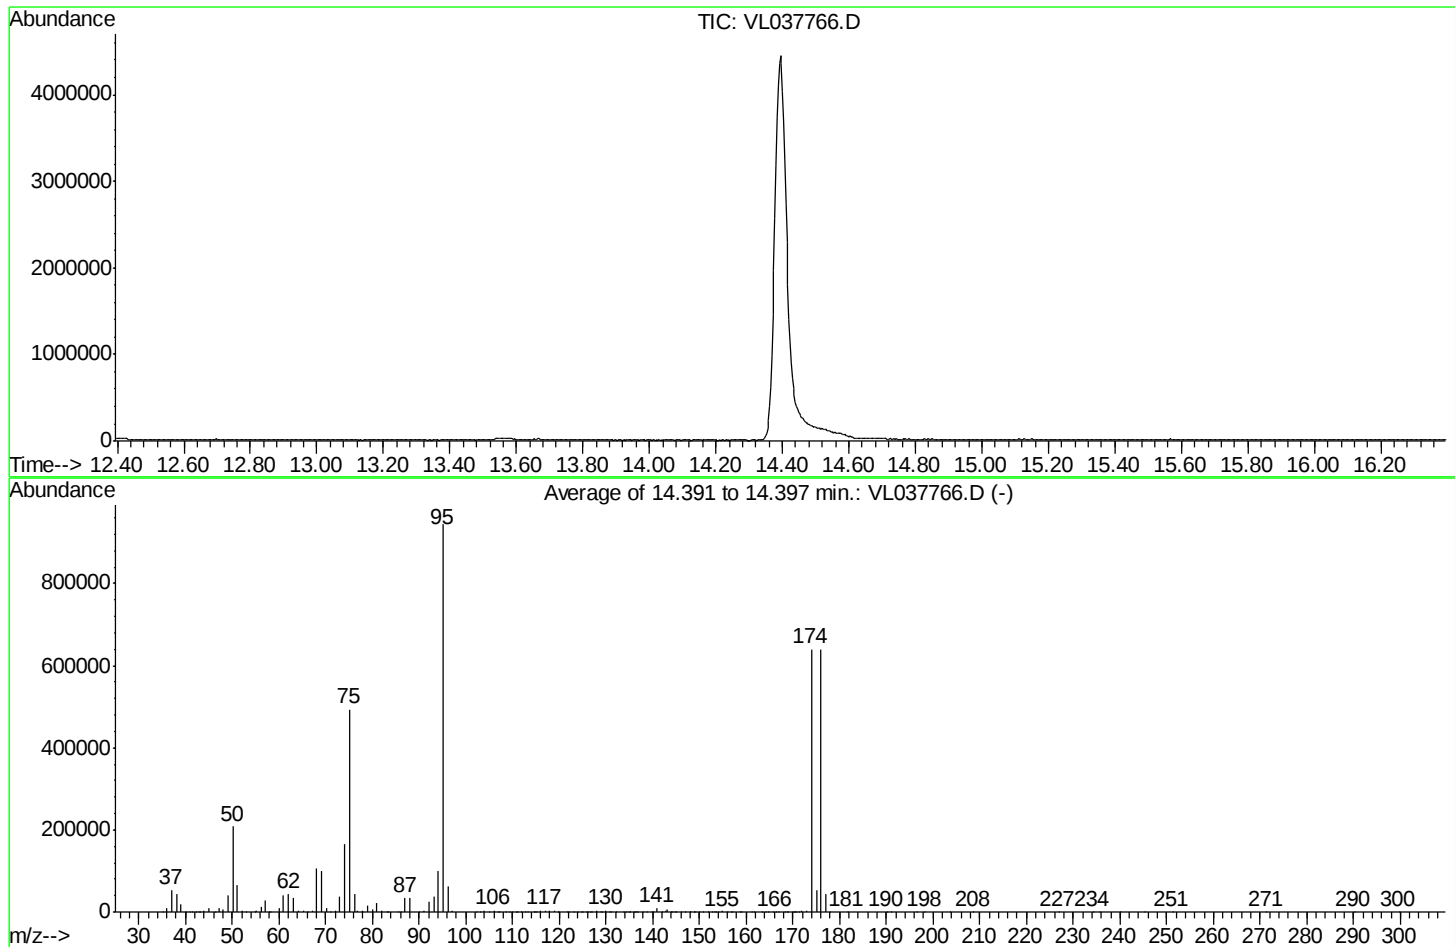

AutoFind: Scans 3609, 3610, 3611; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.0	207509	PASS
75	95	30	66	52.3	494058	PASS
95	95	100	100	100.0	944128	PASS
96	95	5	9	6.7	63653	PASS
173	174	0.00	2	0.4	2305	PASS
174	95	50	120	67.7	639402	PASS
175	174	4	9	8.1	51685	PASS
176	174	93	101	99.8	637930	PASS
177	176	5	9	6.9	44152	PASS