


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL100719\
Data File : VL034222.D
Acq On : 7 Oct 2019 11:32
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091719AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Sep 18 12:53:31 2019
Last Update : Wed Sep 18 12:53:31 2019

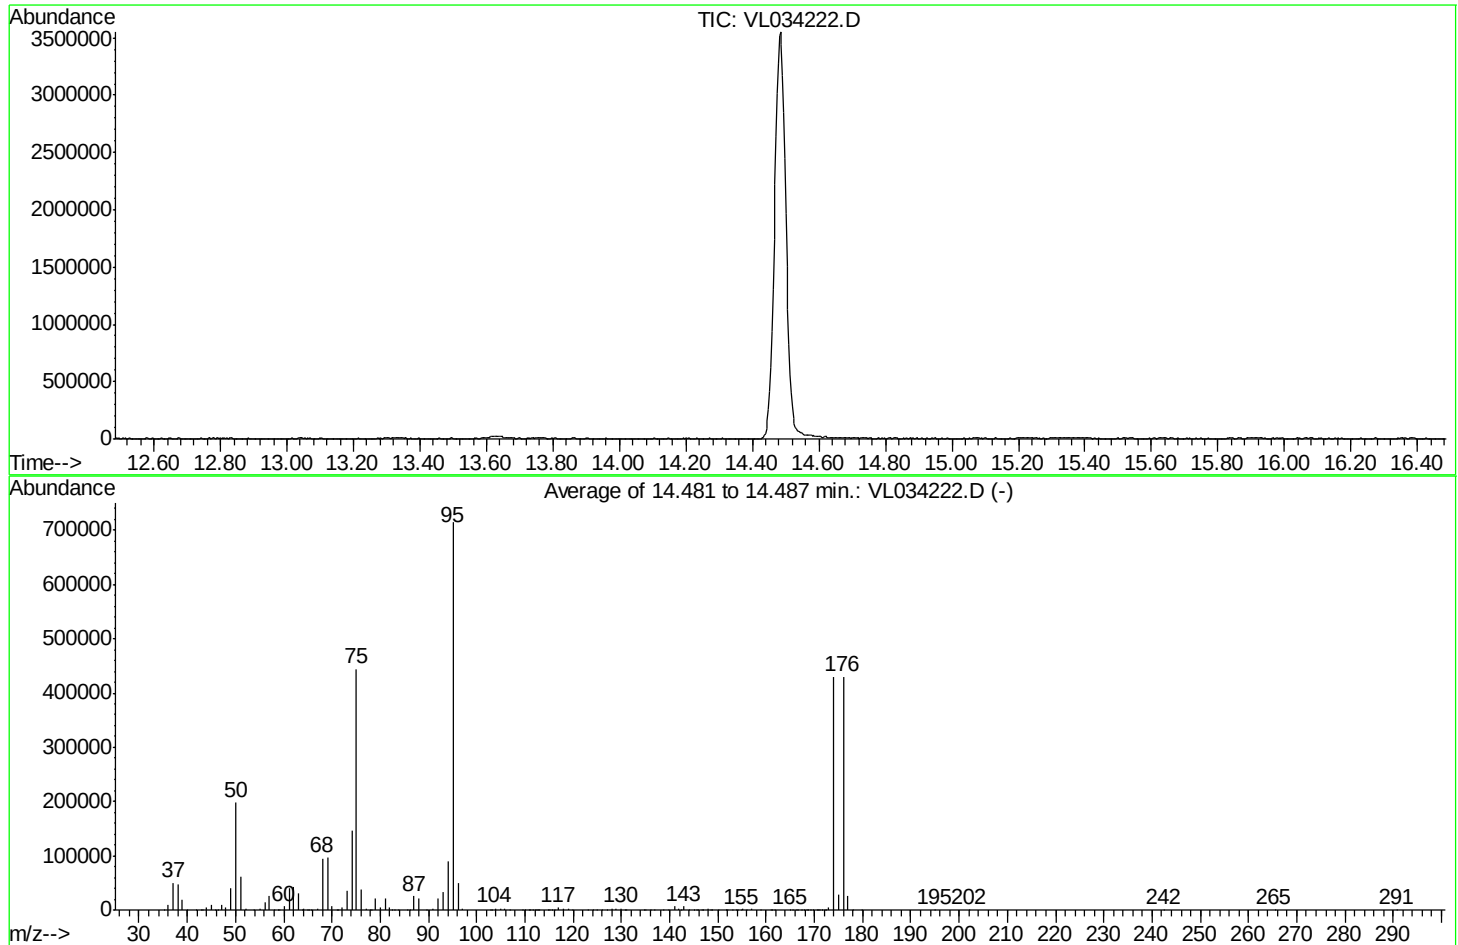

AutoFind: Scans 3637, 3638, 3639; Background Corrected with Scan 3612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.6	197333	PASS
75	95	30	66	62.2	444842	PASS
95	95	100	100	100.0	714688	PASS
96	95	5	9	6.8	48773	PASS
173	174	0.00	2	1.0	4259	PASS
174	95	50	120	60.0	428928	PASS
175	174	4	9	6.8	29098	PASS
176	174	93	101	100.3	430186	PASS
177	176	5	9	6.3	27056	PASS