


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL100819\
Data File : VL034250.D
Acq On : 8 Oct 2019 14:12
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091719AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Sep 18 12:53:31 2019
Last Update : Wed Sep 18 12:53:31 2019

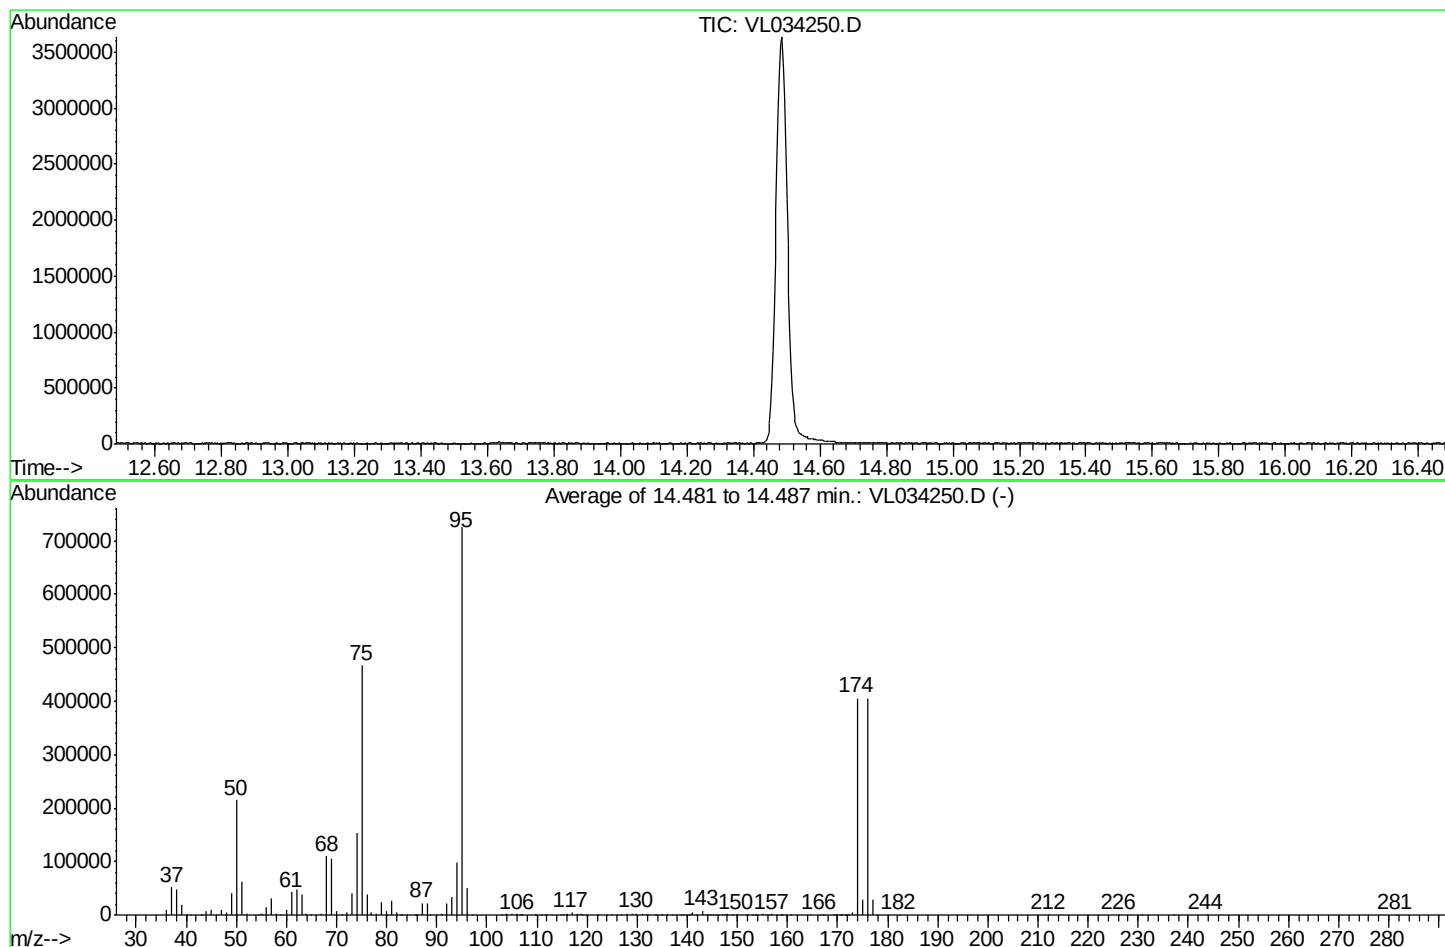

AutoFind: Scans 3637, 3638, 3639; Background Corrected with Scan 3612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	29.7	215402	PASS
75	95	30	66	64.3	466730	PASS
95	95	100	100	100.0	725312	PASS
96	95	5	9	7.1	51205	PASS
173	174	0.00	2	1.0	3920	PASS
174	95	50	120	55.9	405248	PASS
175	174	4	9	7.3	29597	PASS
176	174	93	101	99.7	403904	PASS
177	176	5	9	7.0	28160	PASS