

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL100820\
 Data File : VL035745.D
 Acq On : 8 Oct 2020 14:56
 Operator : SY/AP
 Sample : L4275-01
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFI-EFFLUENT-TANK

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 3 Min Area: 3 % of largest Peak
 Start Thrs: 0.001 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL092320AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Sep 23 07:38:05 2020

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.867	10	25	38	rBV	3617075	6430739	9.15%	1.249%
2	2.983	55	61	76	rVB	1606758	2262198	3.22%	0.439%
3	3.156	96	115	124	rBV	4885802	7006604	9.97%	1.361%
4	3.555	227	239	246	rBV	2142615	2984205	4.25%	0.580%
5	3.851	324	331	349	rVB	526839	844187	1.20%	0.164%
6	4.343	474	484	500	rVB2	938579	1447684	2.06%	0.281%
7	5.012	669	692	705	rBV	4240939	7145133	10.16%	1.388%
8	5.552	847	860	881	rBV	2951225	4763679	6.78%	0.925%
9	5.671	884	897	915	rVV	3120398	5561743	7.91%	1.080%
10	6.899	1254	1279	1301	rBV	8718787	17720662	25.21%	3.442%
11	7.185	1355	1368	1386	rVB	4663533	9077226	12.91%	1.763%
12	9.828	2168	2190	2213	rBV	20058105	53517316	76.13%	10.396%
13	12.105	2872	2898	2909	rBV	5241122	11526047	16.40%	2.239%
14	12.163	2909	2916	2940	rVB2	1416471	3021663	4.30%	0.587%
15	12.732	3075	3093	3111	rBV	2605192	5438203	7.74%	1.056%
16	12.989	3153	3173	3208	rBV	10626648	40338065	57.38%	7.836%
17	13.716	3378	3399	3424	rBV	13136216	32570300	46.33%	6.327%
18	14.442	3605	3625	3654	rBV	5819163	13635773	19.40%	2.649%
19	14.690	3682	3702	3722	rBV	2668719	6053521	8.61%	1.176%
20	15.587	3965	3981	4005	rBV	3807130	8814338	12.54%	1.712%
21	15.799	4026	4047	4058	rBV2	12454106	32566985	46.33%	6.326%
22	15.870	4058	4069	4097	rVB	11693255	29202556	41.54%	5.673%
23	16.027	4097	4118	4144	rBV	14397255	37628180	53.53%	7.309%
24	16.355	4196	4220	4242	rBV	6265493	15159569	21.57%	2.945%
25	16.709	4313	4330	4338	rBV2	524511	1173146	1.67%	0.228%
26	16.802	4338	4359	4401	rVB	24034016	70293870	100.00%	13.655%
27	17.008	4404	4423	4444	rVB2	696653	1898046	2.70%	0.369%
28	17.169	4456	4473	4484	rBV2	313455	724525	1.03%	0.141%
29	17.323	4507	4521	4538	rVB2	307379	744335	1.06%	0.145%
30	17.567	4575	4597	4602	rBV2	1183945	2321999	3.30%	0.451%
31	17.629	4602	4616	4650	rVB	10437708	27294110	38.83%	5.302%
32	17.847	4665	4684	4700	rBV2	358511	839419	1.19%	0.163%
33	18.005	4710	4733	4748	rBV	1787839	4503014	6.41%	0.875%
34	18.349	4821	4840	4852	rBV3	1224427	2794501	3.98%	0.543%

LSC Area Percent Report

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL100820\
Data File : VL035745.D
Acq On : 8 Oct 2020 14:56
Operator : SY/AP
Sample : L4275-01
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFI-EFFLUENT-TANK

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON
Sampling : 3
Start Thrs: 0.001
Stop Thrs : 0
Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL092320AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Sep 23 07:38:05 2020

35	18.426	4852	4864	4882	rVV	1726673	3994580	5.68%	0.776%
36	18.548	4882	4902	4906	rVV	1031704	2219830	3.16%	0.431%
37	18.596	4906	4917	4943	rVV2	3039077	7498761	10.67%	1.457%
38	18.899	4989	5011	5029	rBV2	806783	1921020	2.73%	0.373%
39	19.159	5075	5092	5102	rBV2	1845843	4304740	6.12%	0.836%
40	19.220	5102	5111	5129	rVB2	1940961	4483214	6.38%	0.871%
41	19.387	5147	5163	5179	rBV	4238590	9831985	13.99%	1.910%
42	19.979	5336	5347	5365	rVB3	645799	1462860	2.08%	0.284%
43	20.301	5430	5447	5464	rBV2	1673308	4240412	6.03%	0.824%
44	20.397	5464	5477	5503	rVB2	2054892	5005615	7.12%	0.972%
45	20.927	5621	5642	5653	rBV5	270303	887410	1.26%	0.172%
46	21.243	5717	5740	5753	rBV5	271518	770350	1.10%	0.150%
47	21.329	5753	5767	5788	rVB2	331315	868387	1.24%	0.169%


Sum of corrected areas: 514792705

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL100820\
Data File : VL035745.D
Acq On : 8 Oct 2020 14:56
Operator : SY/AP
Sample : L4275-01
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFI-EFFLUENT-TANK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL092320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Sep 23 07:38:05 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

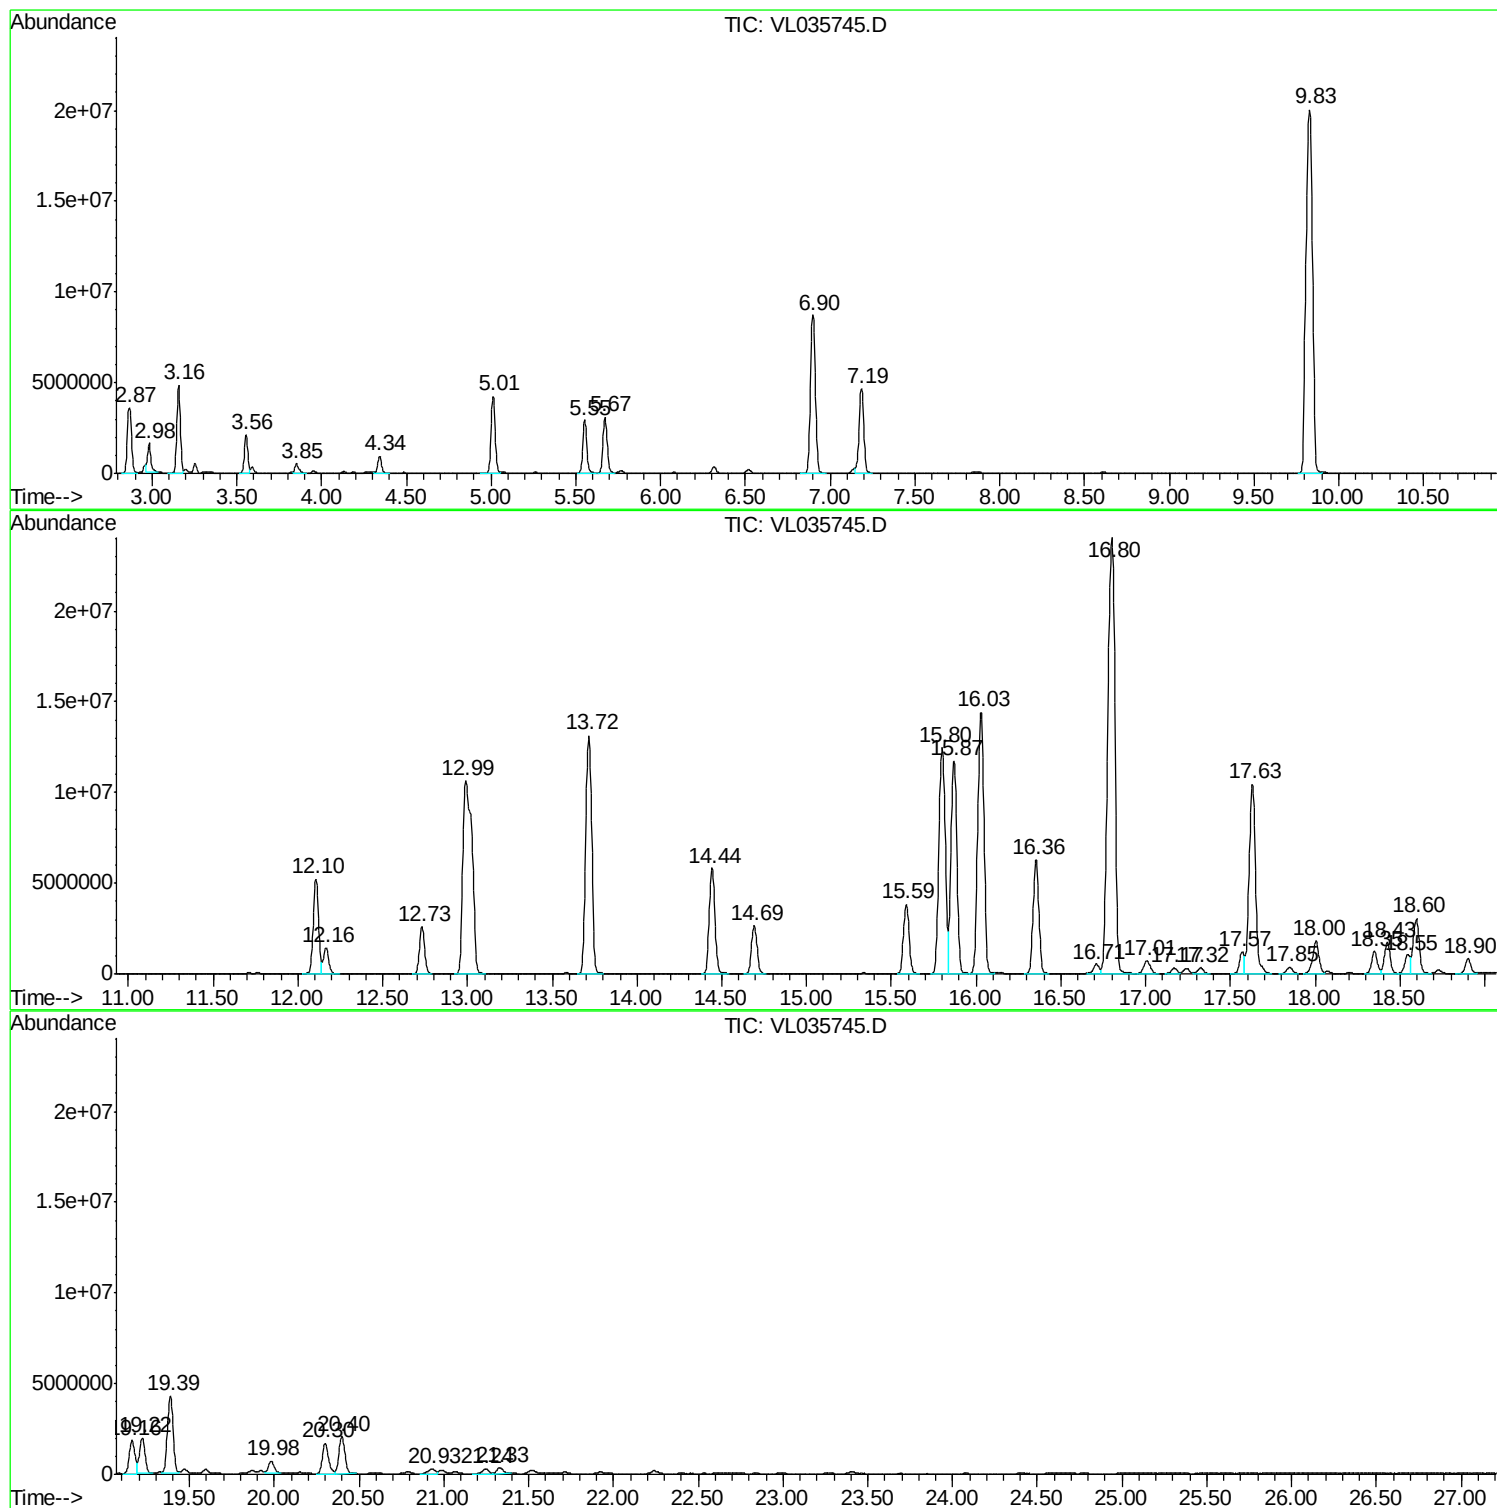

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL100820\
Data File : VL035745.D
Acq On : 8 Oct 2020 14:56
Operator : SY/AP
Sample : L4275-01
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFI-EFFLUENT-TANK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL092320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Sep 23 07:38:05 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL100820\
Data File : VL035745.D
Acq On : 8 Oct 2020 14:56
Operator : SY/AP
Sample : L4275-01
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFI-EFFLUENT-TANK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL092320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Sep 23 07:38:05 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc