


Data Path : W:\HPCHEM1\MSVOA L\DATA\VL100915\
Data File : VL026171.D
Acq On : 9 Oct 2015 10:21
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL100915AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Oct 09 16:23:14 2015
Last Update : Fri Oct 09 16:23:14 2015

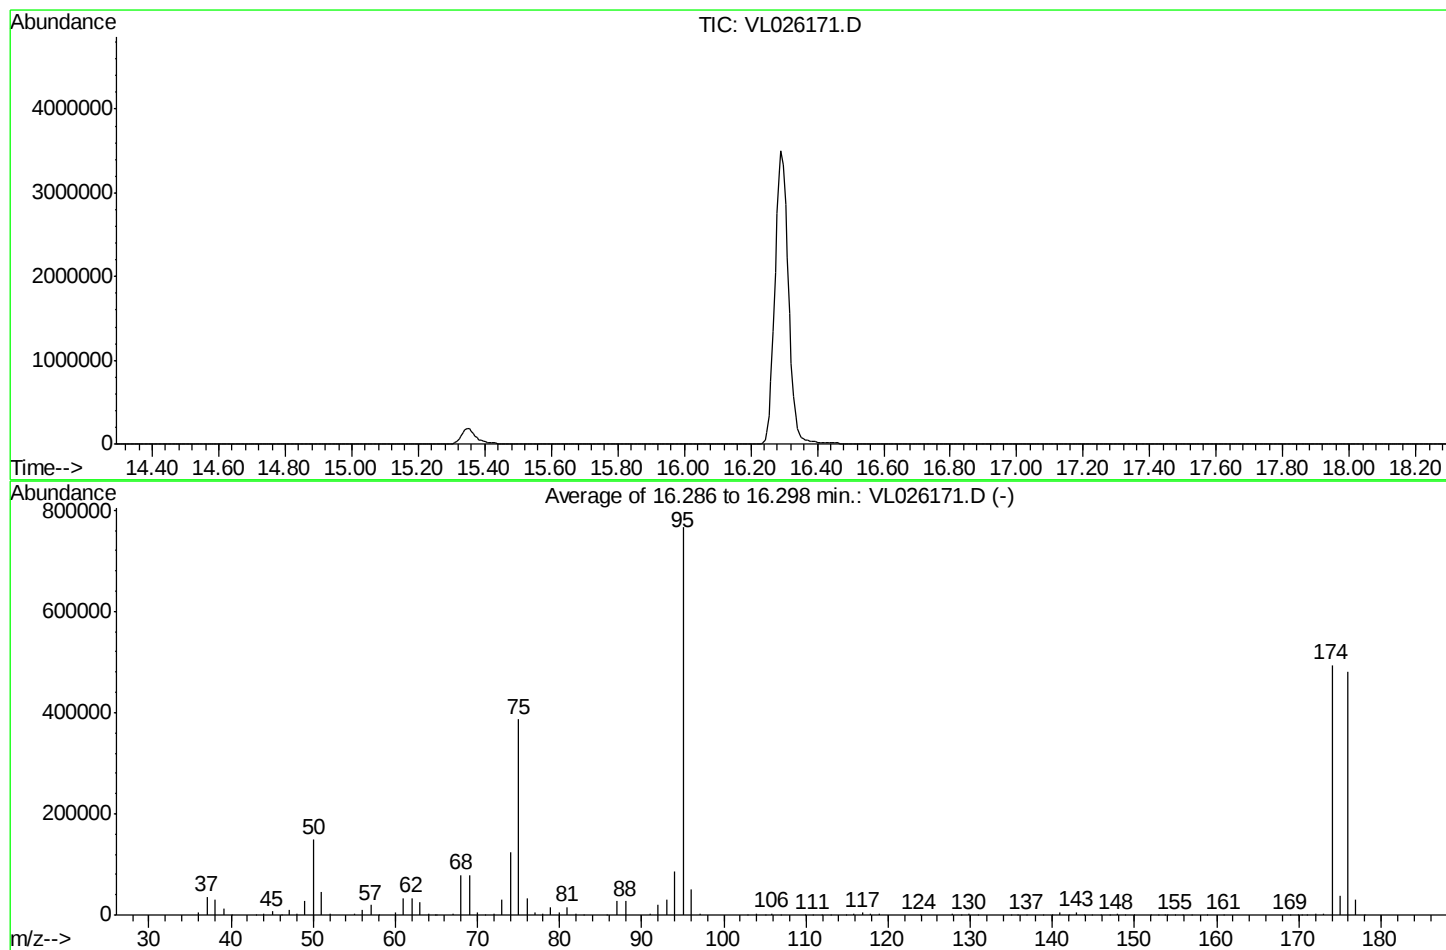

AutoFind: Scans 2165, 2166, 2167; Background Corrected with Scan 2148

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	19.3	148224	PASS
75	95	30	66	50.5	386645	PASS
95	95	100	100	100.0	766165	PASS
96	95	5	9	6.7	51570	PASS
173	174	0.00	2	0.7	3666	PASS
174	95	50	120	64.5	494165	PASS
175	174	4	9	7.6	37544	PASS
176	174	93	101	97.1	480064	PASS
177	176	5	9	6.4	30901	PASS