


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101024\
Data File : VL041633.D
Acq On : 10 Oct 2024 8:26
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091624AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Sep 17 09:12:21 2024

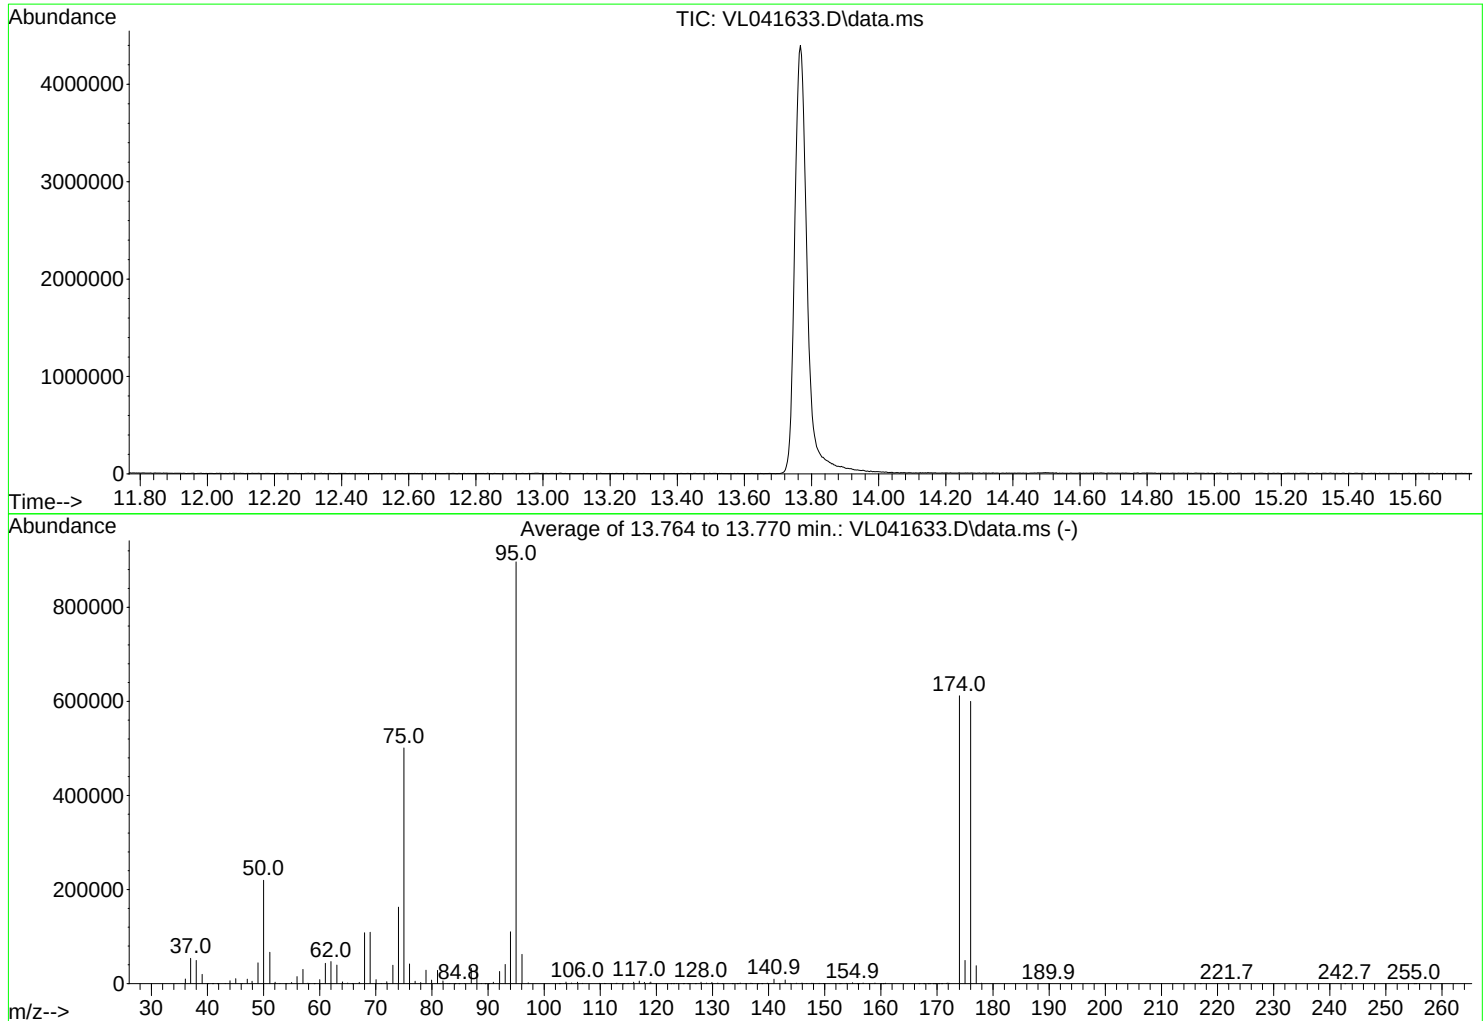

AutoFind: Scans 3471, 3472, 3473; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.5	219669	PASS
75	95	30	66	55.9	500971	PASS
95	95	100	100	100.0	896555	PASS
96	95	5	9	7.0	62421	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.3	611947	PASS
175	174	4	9	8.1	49312	PASS
176	174	93	101	98.1	600021	PASS
177	176	5	9	6.4	38163	PASS

Average of 13.764 to 13.770 min.: VL041633.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9871	46.20	348	57.00	30237	67.05	270
37.00	53869	47.10	9397	57.90	911	68.00	10828
38.00	49395	47.95	5226	58.20	333	69.00	10911
39.05	19653	49.00	44152	59.00	62	70.05	860
40.00	126	50.00	219669	60.00	8383	70.95	294
40.90	85	51.10	66595	61.00	43061	71.95	3968
41.80	107	52.05	2923	62.00	46885	73.05	38976
43.15	306	52.90	369	63.05	39432	74.05	162645
44.00	6188	53.95	126	64.05	3661	75.00	500971
45.05	10578	55.00	2513	65.00	1528	76.00	41803
45.95	326	55.95	15140	65.80	117	77.00	4987

Average of 13.764 to 13.770 min.: VL041633.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.00	2339	88.00	30464	102.70	64	112.95	878
78.95	28467	88.80	298	102.95	414	114.10	59
79.95	7669	89.50	57	103.90	3522	114.95	822
81.00	28147	90.10	78	104.90	1500	115.95	3054
81.95	5913	90.95	3159	105.95	3173	116.95	5439
82.85	371	92.05	25829	106.85	813	117.85	2854
83.15	435	93.05	40917	109.85	607	118.80	1384
84.10	68	94.00	110291	110.80	834	119.00	3397
84.80	50	95.00	896555	111.00	285	121.70	200
85.85	500	96.05	62421	111.90	789	122.60	65
87.00	32909	97.15	1854	112.80	208	123.05	167

Average of 13.764 to 13.770 min.: VL041633.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.60	196	131.75	106	140.95	9515	150.00	267
123.90	247	133.55	126	141.90	686	151.90	302
124.80	84	134.40	68	142.95	7881	152.65	167
125.00	327	134.70	299	143.85	581	153.05	301
125.60	124	134.95	1358	144.95	996	153.90	748
126.00	391	135.90	160	145.95	1332	154.95	2201
126.95	164	136.85	1026	146.80	367	155.80	154
127.95	3018	137.10	407	147.70	1157	156.00	130
128.95	1472	138.10	134	148.00	567	156.85	1555
129.90	2906	138.80	189	149.00	725	157.85	330
130.95	1234	139.75	969	149.80	505	158.95	1293

Average of 13.764 to 13.770 min.: VL041633.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.00	119	170.80	153	216.90	51		
160.40	111	171.00	232	221.70	77		
160.80	939	171.70	584	242.70	58		
166.80	70	171.95	1388	255.00	99		
167.65	116	172.20	599	255.30	82		
168.40	70	174.00	611947				
168.70	121	175.00	49312				
169.35	164	176.00	600021				
169.70	118	177.00	38163				
169.90	246	177.95	936				
170.30	103	189.90	64				

Instrument :

MSVOA_L

ClientSampleId :

BFB