


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL101118\
Data File : VL032598.D
Acq On : 11 Oct 2018 9:02
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL092418AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 01 06:49:26 2018
Last Update : Mon Oct 01 06:49:26 2018

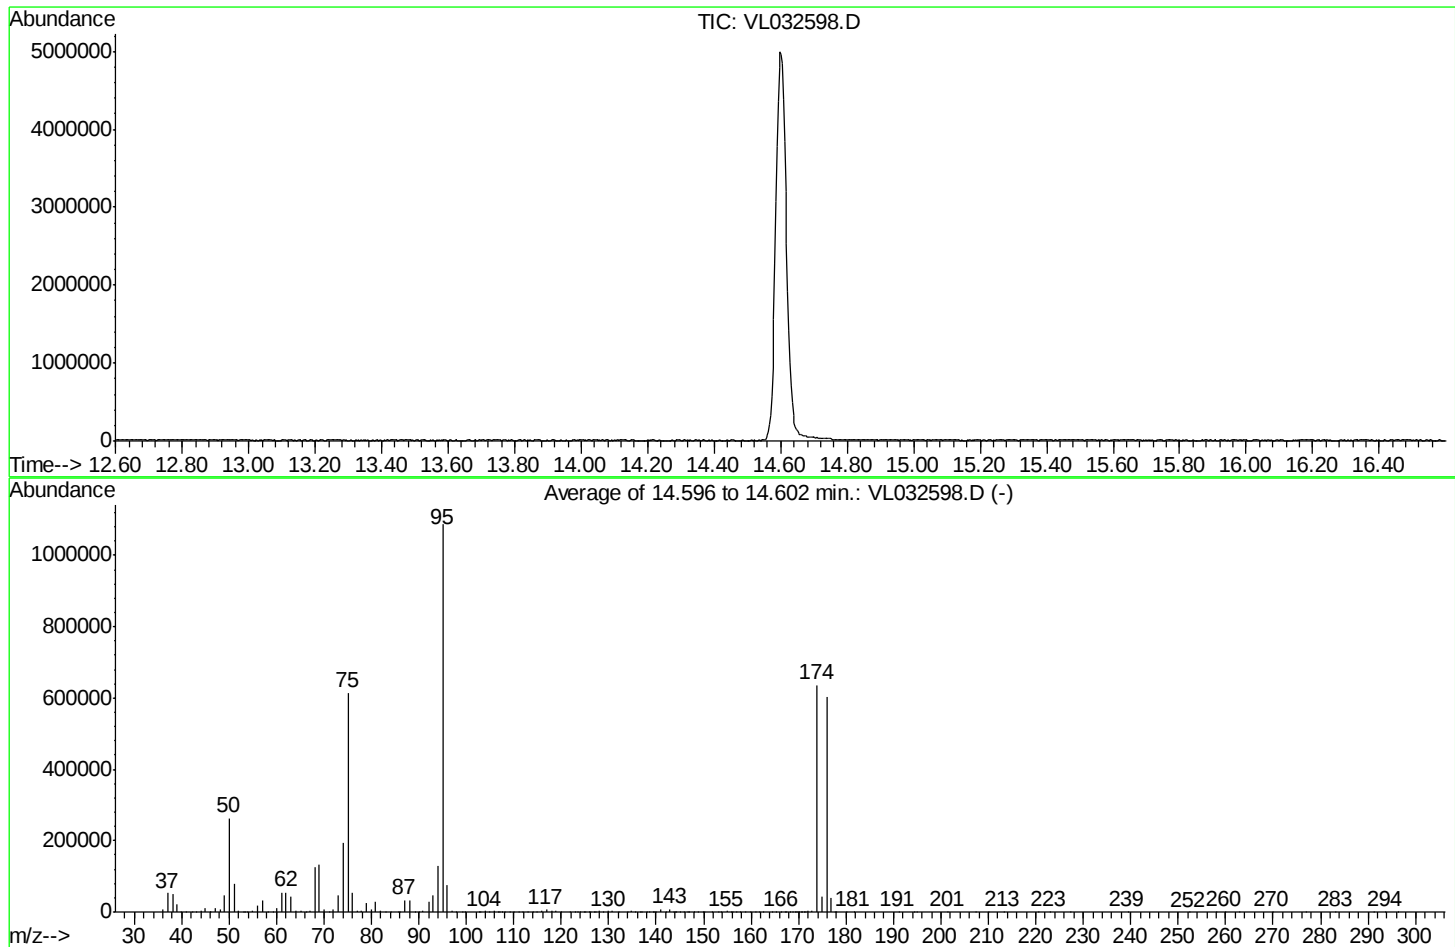

AutoFind: Scans 3626, 3627, 3628; Background Corrected with Scan 3603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.1	262442	PASS
75	95	30	66	56.5	613909	PASS
95	95	100	100	100.0	1087082	PASS
96	95	5	9	6.9	75252	PASS
173	174	0.00	2	0.8	5043	PASS
174	95	50	120	58.6	636629	PASS
175	174	4	9	7.0	44802	PASS
176	174	93	101	95.0	604757	PASS
177	176	5	9	6.3	37826	PASS