
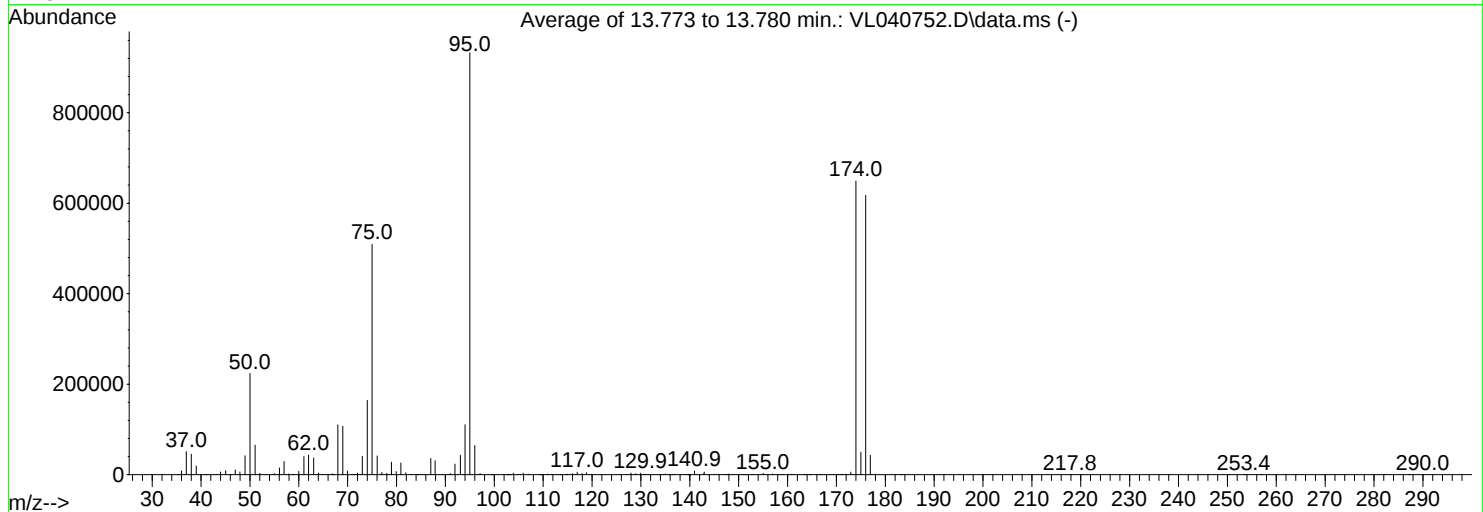


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101123\
Data File : VL040752.D
Acq On : 11 Oct 2023 10:43
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101123AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Oct 12 00:21:08 2023

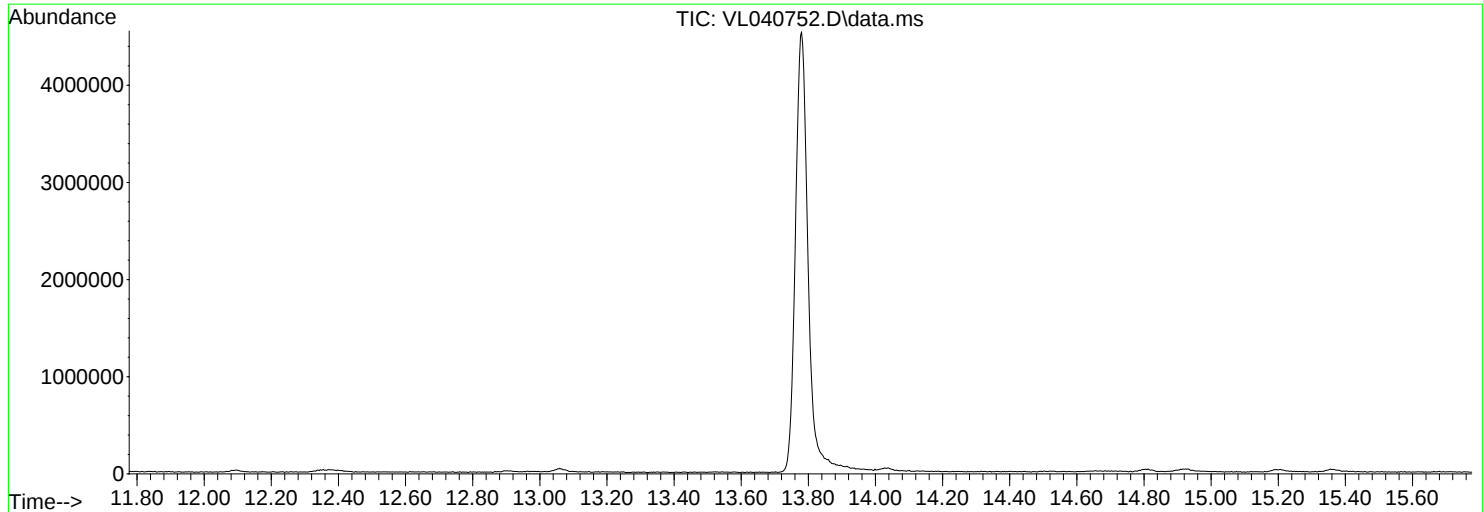

AutoFind: Scans 3474, 3475, 3476; Background Corrected with Scan 3438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.0	223794	PASS
75	95	30	66	54.6	508928	PASS
95	95	100	100	100.0	932331	PASS
96	95	5	9	6.9	64457	PASS
173	174	0.00	2	0.9	5668	PASS
174	95	50	120	69.6	649067	PASS
175	174	4	9	7.7	49693	PASS
176	174	93	101	95.2	617685	PASS
177	176	5	9	6.9	42781	PASS

Average of 13.773 to 13.780 min.: VL040752.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.30	94	45.90	168	56.05	14915	67.05	161
36.00	8628	46.20	247	57.00	29199	68.00	11017
37.00	50851	47.00	10428	57.95	1388	69.00	10723
38.00	45267	47.95	6135	58.80	131	69.95	834
39.00	19238	49.00	41853	60.00	7279	70.90	296
39.95	161	50.00	223794	61.05	40141	71.30	133
41.00	139	51.05	65223	62.00	43259	72.00	3593
41.95	197	52.05	2829	63.05	36824	73.00	40571
43.20	842	53.10	194	64.05	3603	74.00	164075
44.00	5899	53.85	540	64.95	384	75.00	508928
45.05	8749	55.05	2276	66.85	1936	76.05	41475

Average of 13.773 to 13.780 min.: VL040752.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	4774	87.90	30648	99.90	71	110.95	1018
78.00	3212	89.40	272	102.60	182	111.75	816
78.95	27432	90.90	721	102.80	144	112.90	495
79.95	6726	91.05	2055	103.20	160	113.10	305
80.90	25840	91.95	23528	103.90	3405	113.60	129
81.90	4297	93.05	42677	104.95	890	114.00	201
83.00	731	94.00	110335	105.90	3492	114.60	185
84.30	87	95.00	932331	106.95	1052	114.95	1024
85.05	205	96.00	64457	109.40	81	115.70	689
85.80	799	97.10	2340	109.60	100	116.00	2676
87.00	35672	99.40	64	110.00	305	116.95	5272

Average of 13.773 to 13.780 min.: VL040752.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.95	2474	129.90	3141	136.95	1104	143.80	250
118.85	4177	130.70	337	138.00	63	144.00	312
119.90	230	130.90	672	139.00	354	145.00	911
121.70	204	131.80	58	139.20	201	145.85	1155
122.75	309	133.85	173	139.60	189	147.00	702
123.95	810	134.10	149	140.00	136	147.50	296
125.00	270	134.70	292	140.95	7924	147.70	431
125.85	586	135.00	1337	141.90	656	147.95	1337
126.90	242	135.70	76	142.10	382	148.75	381
127.95	3415	136.00	437	142.80	1859	149.00	344
128.95	2176	136.30	128	142.95	5601	149.85	740

Average of 13.773 to 13.780 min.: VL040752.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
150.10	398	158.75	522	170.40	679	183.20	54
150.90	189	159.10	217	170.90	110	217.80	62
151.40	54	160.00	145	171.30	647	250.20	51
152.05	605	160.85	1034	171.85	1095	253.40	56
152.70	257	161.10	204	172.20	594	256.90	52
153.05	478	163.40	62	172.95	5668	282.00	57
153.90	335	164.55	159	174.00	649067	287.10	62
155.00	2745	166.70	122	175.00	49693	290.00	63
155.95	620	167.65	383	176.00	617685		
156.95	1459	168.80	357	176.95	42781		
157.90	112	169.40	558	177.95	1596		