


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL101220\
 Data File : VL035755.D
 Acq On : 12 Oct 2020 9:04
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL092320AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Sep 23 07:38:05 2020
 Last Update : Wed Sep 23 07:38:05 2020

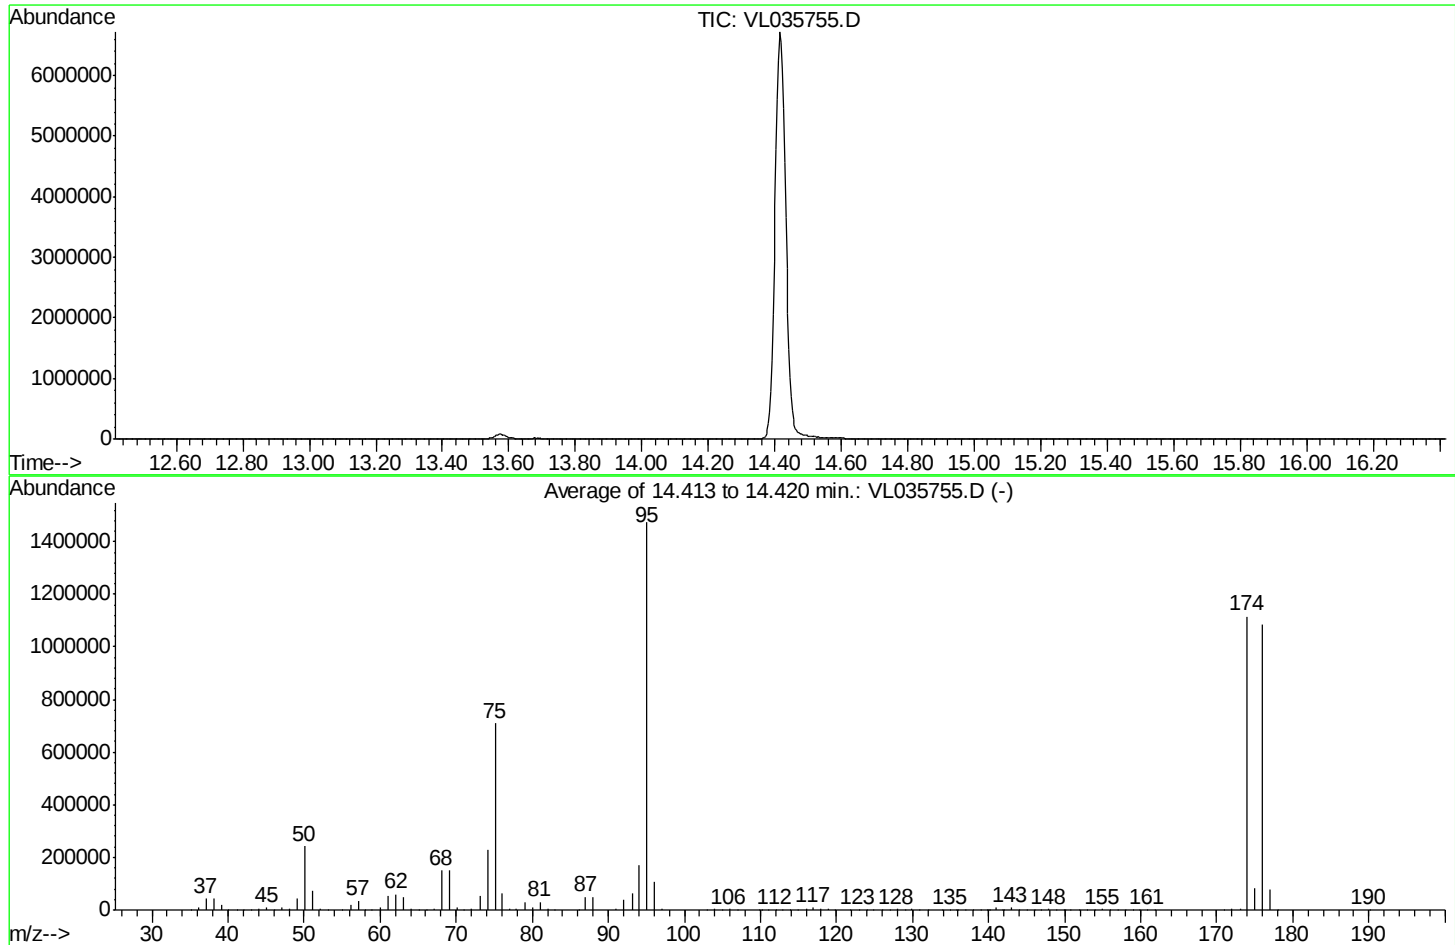

AutoFind: Scans 3616, 3617, 3618; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	16.5	242816	PASS
75	95	30	66	48.1	708416	PASS
95	95	100	100	100.0	1473536	PASS
96	95	5	9	7.2	106421	PASS
173	174	0.00	2	0.5	5812	PASS
174	95	50	120	75.7	1114965	PASS
175	174	4	9	7.5	83954	PASS
176	174	93	101	97.2	1084074	PASS
177	176	5	9	7.0	75800	PASS