

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL101221\
 Data File : VL037838.D
 Acq On : 12 Oct 2021 20:34
 Operator : SY/AP
 Sample : M4079-08
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 COP20

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 3
 Start Thrs: 0.001
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.873	13	27	65	rBV	9441301	36623479	100.00%	24.974%
2	3.198	119	128	153	rBV	1042807	2008107	5.48%	1.369%
3	3.308	153	162	172	rVV	644980	1044273	2.85%	0.712%
4	3.841	319	328	356	rBV	2234696	4575702	12.49%	3.120%
5	4.340	474	483	498	rBV2	692765	1188350	3.24%	0.810%
6	5.243	753	764	788	rVB2	407255	848694	2.32%	0.579%
7	5.664	882	895	913	rBV5	2357401	5713027	15.60%	3.896%
8	5.748	913	921	934	rVB3	282708	571777	1.56%	0.390%
9	7.169	1346	1363	1384	rBV	4121096	8932144	24.39%	6.091%
10	7.471	1445	1457	1476	rBV4	196839	564614	1.54%	0.385%
11	10.423	2359	2375	2386	rBV5	210515	527424	1.44%	0.360%
12	11.214	2603	2621	2638	rBV3	677301	1607894	4.39%	1.096%
13	11.683	2750	2767	2769	rBV2	245265	396712	1.08%	0.271%
14	12.076	2868	2889	2915	rBV2	4216830	10428994	28.48%	7.112%
15	12.339	2957	2971	2985	rVB5	189133	446488	1.22%	0.304%
16	12.696	3057	3082	3099	rBV6	171621	500197	1.37%	0.341%
17	12.957	3148	3163	3164	rBV	302983	402070	1.10%	0.274%
18	14.407	3595	3614	3656	rBV2	3927606	11151725	30.45%	7.604%
19	15.304	3882	3893	3909	rVB8	221555	572084	1.56%	0.390%
20	16.111	4129	4144	4157	rVB3	487851	1163999	3.18%	0.794%
21	16.510	4255	4268	4278	rBV6	219577	556868	1.52%	0.380%
22	16.966	4386	4410	4426	rBV2	924492	2749103	7.51%	1.875%
23	17.117	4448	4457	4473	rVB7	183945	508174	1.39%	0.347%
24	17.256	4488	4500	4516	rBV8	146717	379923	1.04%	0.259%
25	17.538	4574	4588	4605	rBV6	274906	872831	2.38%	0.595%
26	17.674	4613	4630	4632	rBV5	263273	473424	1.29%	0.323%
27	17.928	4689	4709	4737	rBV3	1758330	4811906	13.14%	3.281%
28	18.165	4764	4783	4799	rBV2	718994	1968748	5.38%	1.343%
29	18.349	4819	4840	4879	rBV2	3605019	11065725	30.21%	7.546%
30	18.702	4936	4950	4962	rBV4	332852	891495	2.43%	0.608%
31	18.805	4962	4982	4989	rVV3	562923	1745416	4.77%	1.190%
32	18.895	4992	5010	5025	rVV2	2712364	8945811	24.43%	6.100%
33	18.956	5028	5029	5042	rVV3	816963	1077645	2.94%	0.735%
34	19.053	5042	5059	5086	rVV2	2013630	5786187	15.80%	3.946%

LSC Area Percent Report

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL101221\
Data File : VL037838.D
Acq On : 12 Oct 2021 20:34
Operator : SY/AP
Sample : M4079-08
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
COP20

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 3 Min Area: 3 % of largest Peak
Start Thrs: 0.001 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

35	19.201	5086	5105	5120	rVB8	446769	1207515	3.30%	0.823%
36	19.445	5161	5181	5197	rBV4	1639957	5332765	14.56%	3.636%
37	19.500	5197	5198	5216	rVB5	454997	704021	1.92%	0.480%
38	19.725	5266	5268	5282	rVV5	293546	619542	1.69%	0.422%
39	19.808	5282	5294	5307	rVB6	385724	982641	2.68%	0.670%
40	19.969	5328	5344	5347	rBV6	281469	584221	1.60%	0.398%
41	20.034	5363	5364	5381	rVB3	520057	722750	1.97%	0.493%
42	20.181	5394	5410	5429	rVB7	192917	621368	1.70%	0.424%
43	20.397	5466	5477	5494	rVB6	198464	597554	1.63%	0.407%
44	21.468	5791	5810	5834	rBV2	1054534	3482347	9.51%	2.375%
45	24.808	6836	6849	6864	rBV5	315555	691811	1.89%	0.472%


Sum of corrected areas: 146647545

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL101221\
Data File : VL037838.D
Acq On : 12 Oct 2021 20:34
Operator : SY/AP
Sample : M4079-08
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P20

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

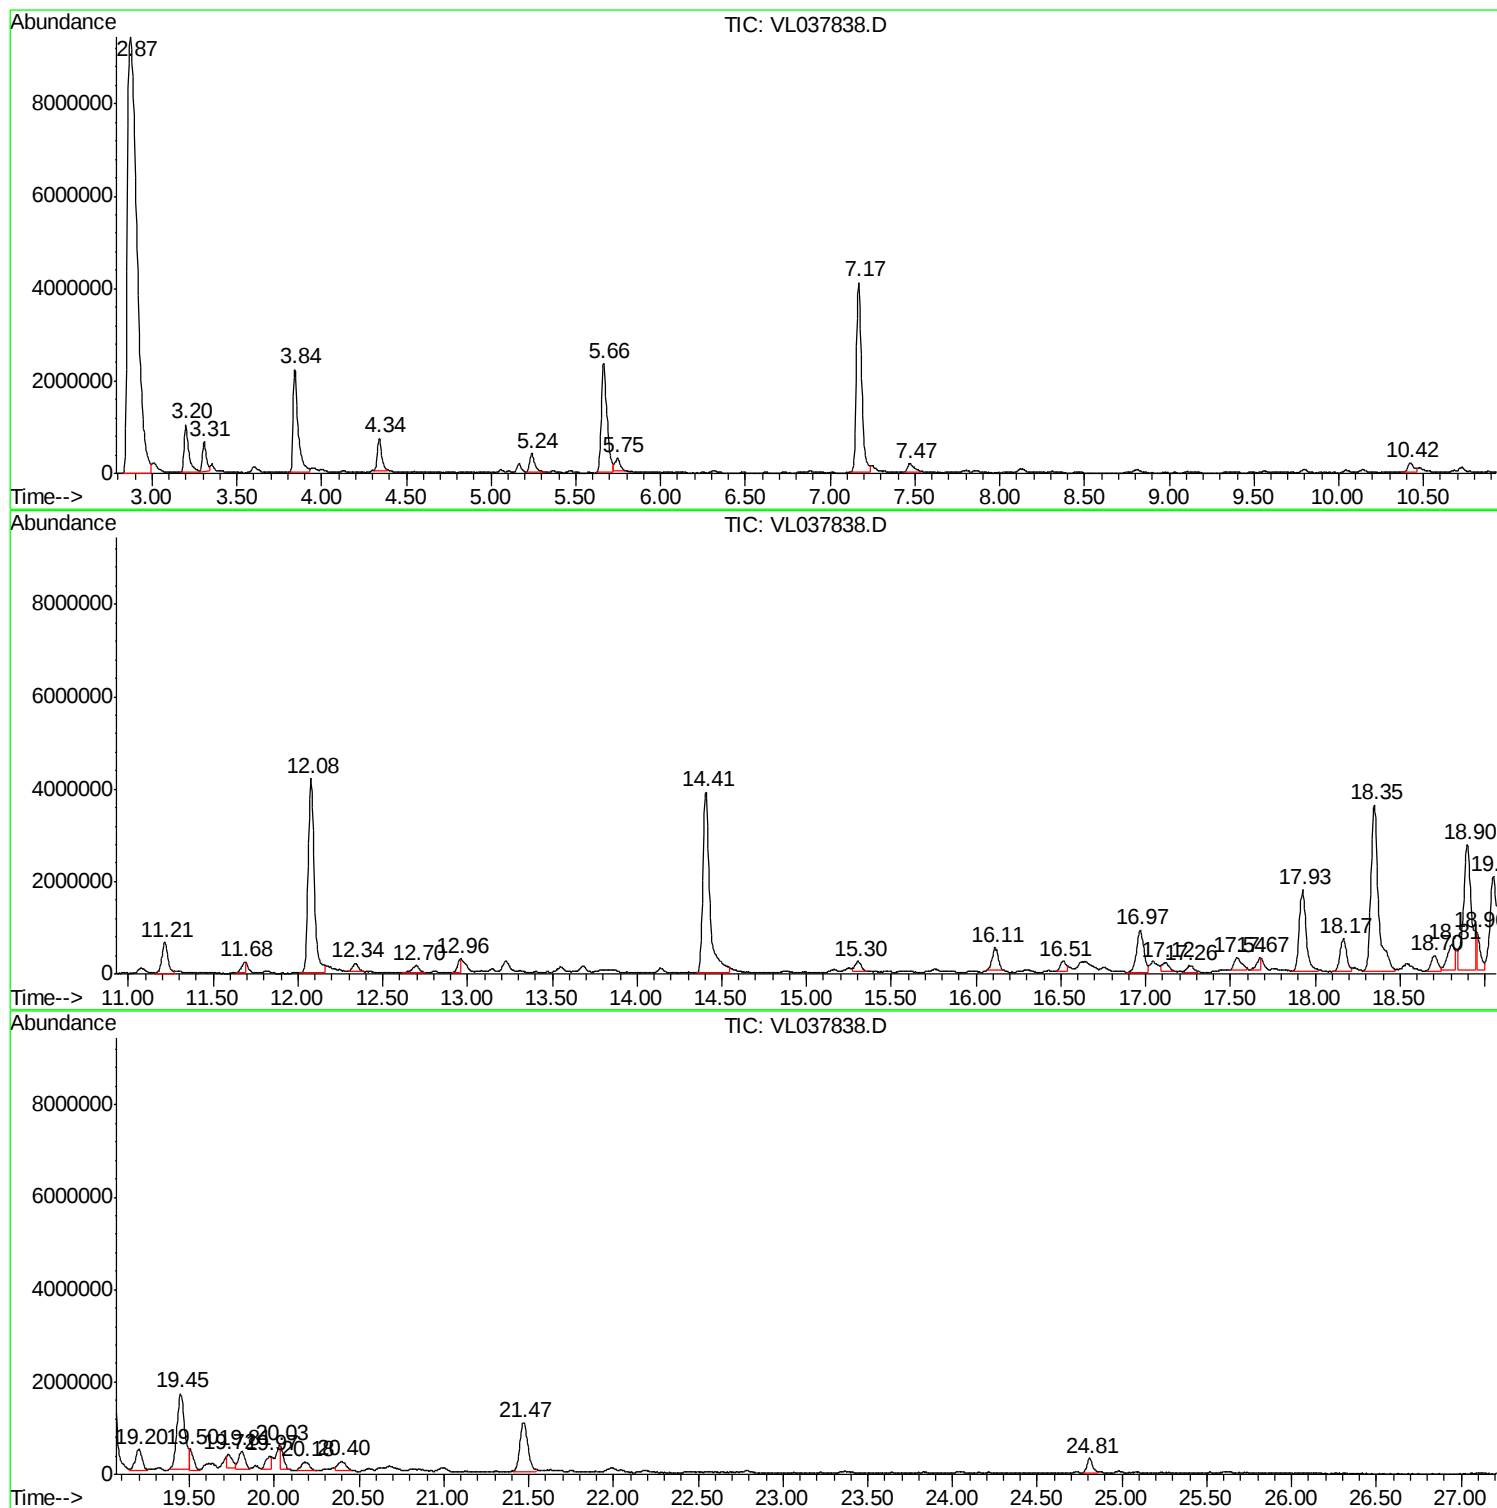

Data_Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL101221\
Data_File : VL037838.D
Acq_On : 12_Oct_2021_ 20:344
Operator : SY/APP
Sample : M4079-088
Misc : 400mL/MSVOA.LL
ALS_Vial : 1_ Sample_Multiplier: 11

Instrument :
MSVOA.L
ClientSampleId :
COP20

Quant_Method : Z:\V0ASRV\HPCHEM1\MSVOA.L\METHODS\VL100421AIR.MM
Quant_Title : AIR ANALYSIS BY METHOD TO-15_ Instrument: MSVOA.L Mon_Oct_04_17:43:54_2021

TIC_Library : C:\DATABASE\NIST20.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
