


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL101221\
 Data File : VL037827.D
 Acq On : 12 Oct 2021 11:18
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021
 Last Update : Mon Oct 04 17:43:54 2021

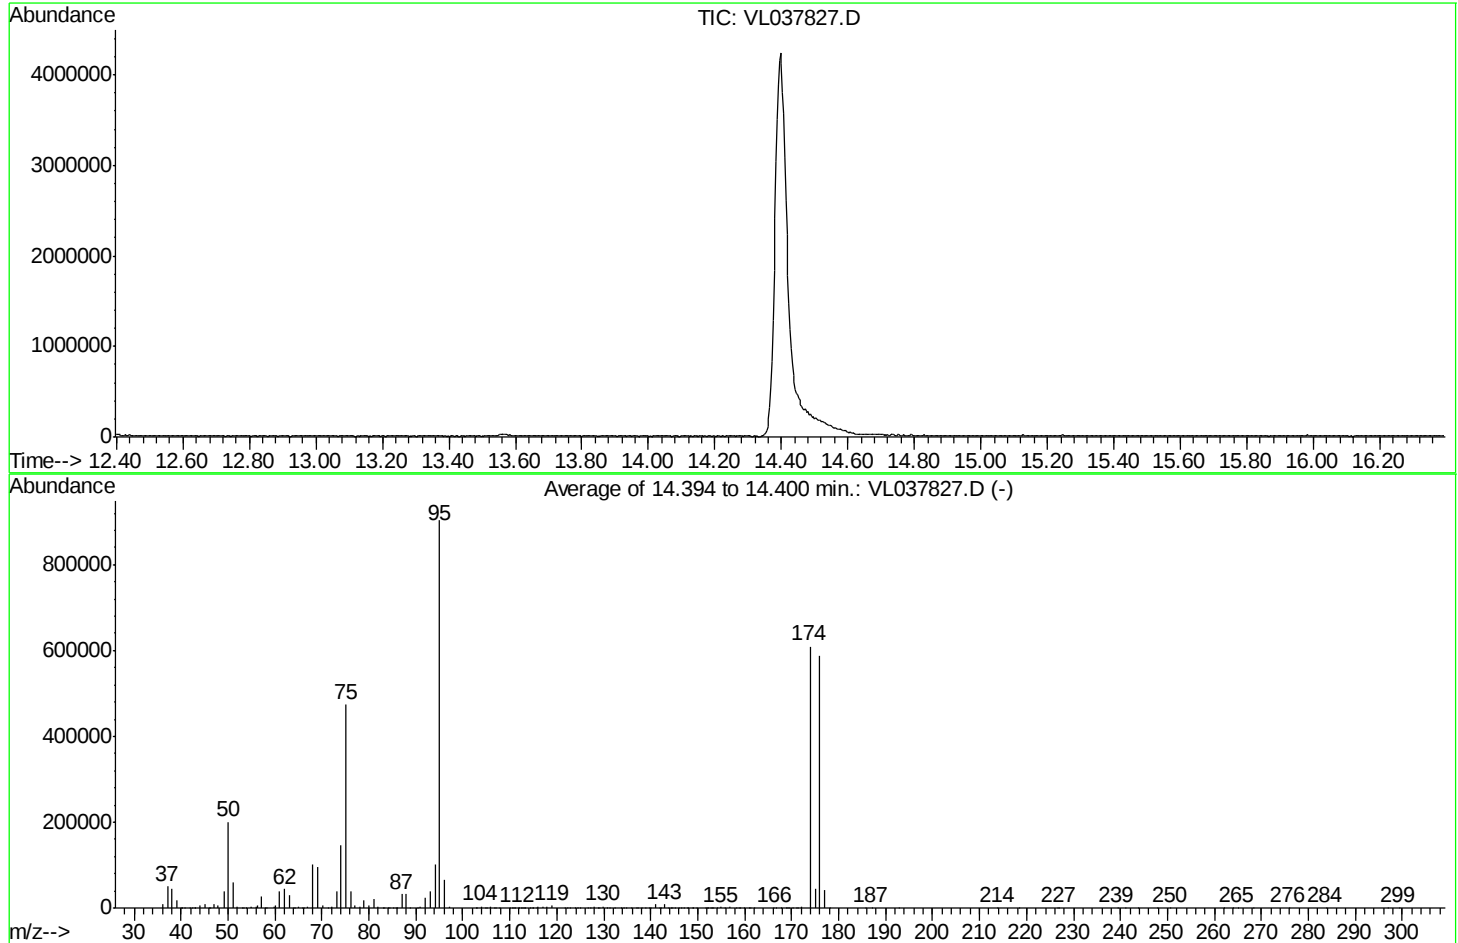

AutoFind: Scans 3610, 3611, 3612; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.2	200640	PASS
75	95	30	66	52.4	473536	PASS
95	95	100	100	100.0	903402	PASS
96	95	5	9	7.2	65016	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.4	608938	PASS
175	174	4	9	7.5	45792	PASS
176	174	93	101	96.7	588672	PASS
177	176	5	9	7.0	41477	PASS