
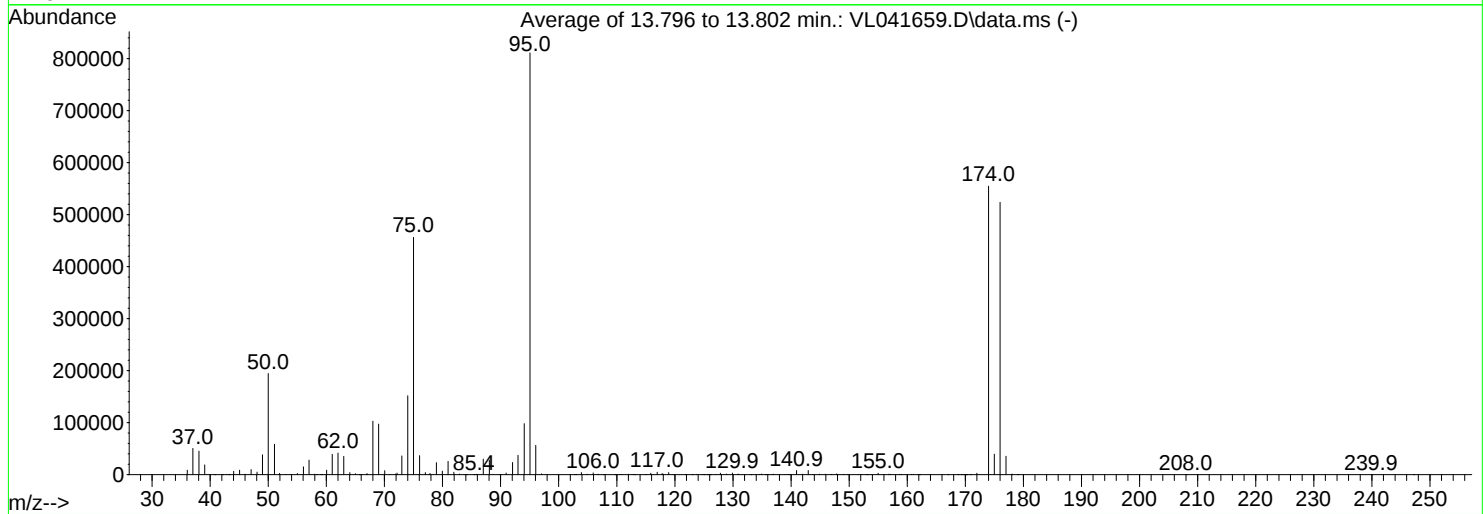


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101424\
Data File : VL041659.D
Acq On : 14 Oct 2024 8:23
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091624AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Sep 17 09:12:21 2024

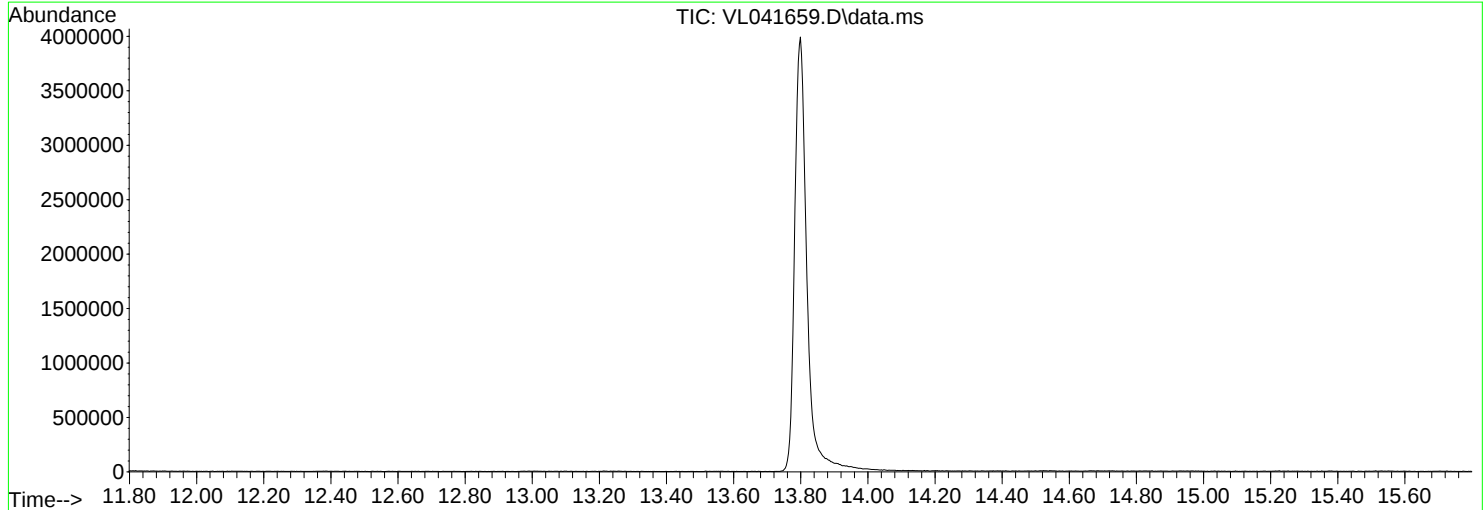

AutoFind: Scans 3481, 3482, 3483; Background Corrected with Scan 3456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.0	194560	PASS
75	95	30	66	56.3	456469	PASS
95	95	100	100	100.0	811243	PASS
96	95	5	9	7.0	56400	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.4	554837	PASS
175	174	4	9	7.1	39429	PASS
176	174	93	101	94.4	523797	PASS
177	176	5	9	6.7	35344	PASS

Average of 13.796 to 13.802 min.: VL041659.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8726	46.00	897	57.00	27944	65.70	15
37.00	50475	47.05	9774	57.95	881	66.05	31
38.05	45219	48.05	5048	58.30	173	66.90	111
39.05	18800	49.00	38032	59.00	350	67.05	157
39.95	607	50.00	194560	59.20	119	68.00	102787
40.80	104	51.05	58525	60.05	8533	69.00	97320
42.10	111	51.95	2534	61.00	39237	70.05	7764
42.85	516	52.95	226	62.00	41453	70.95	312
43.20	160	53.85	274	63.00	34968	71.90	1322
44.05	6589	55.00	2132	64.05	4089	72.15	3120
45.05	8520	56.05	15235	65.00	2010	73.00	36160

Average of 13.796 to 13.802 min.: VL041659.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.00	151701	84.10	86	96.05	56400	110.50	229
75.00	456469	85.40	88	97.05	1587	110.90	757
76.05	36739	85.90	1002	102.70	312	112.00	936
77.05	3976	87.00	29853	102.90	96	112.85	489
77.85	2536	88.05	28061	103.90	3937	113.10	158
78.95	22952	89.90	74	104.90	837	114.90	470
79.95	6923	90.95	3126	105.95	3488	115.10	243
80.95	25715	92.05	23480	106.80	807	115.85	2730
81.95	4777	93.00	37187	107.70	120	116.95	4608
82.90	1169	94.05	98237	109.70	165	117.80	2029
83.85	183	95.05	811243	110.00	365	118.00	806

Average of 13.796 to 13.802 min.: VL041659.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	4048	128.90	1161	136.95	808	146.95	509
119.80	63	129.90	3073	138.95	327	147.85	1706
121.85	175	130.90	1337	139.50	241	149.05	540
122.95	29	131.95	173	139.70	241	149.80	339
123.80	542	133.10	153	140.00	243	150.05	551
124.80	208	133.85	233	140.95	8057	151.55	296
125.00	157	134.60	259	141.95	1087	152.05	499
125.60	188	134.95	1240	142.95	7874	152.90	275
126.10	142	135.60	109	143.80	359	153.10	78
127.05	297	136.10	252	144.90	954	153.75	281
127.85	2760	136.70	454	145.90	993	155.00	2754

Average of 13.796 to 13.802 min.: VL041659.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.10	299	168.75	164	178.05	1123		
156.85	1084	169.30	165	179.00	55		
157.10	610	169.75	167	208.00	53		
157.95	348	170.10	89	239.90	78		
158.65	441	170.30	172	247.20	66		
159.00	759	170.90	162				
160.75	510	172.00	2804				
161.10	259	174.00	554837				
161.80	195	175.00	39429				
162.10	109	176.00	523797				
167.00	99	177.00	35344				