

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101525\
 Data File : VL043118.D
 Acq On : 15 Oct 2025 11:39
 Operator : SY/MD
 Sample : VIBLK
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VIBLK

Quant Time: Oct 16 01:16:19 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Wed Oct 15 02:12:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	90815	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	293345	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	256803	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.377	95	203144	10.177	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.800%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101525\
Data File : VL043118.D
Acq On : 15 Oct 2025 11:39
Operator : SY/MD
Sample : VIBLK
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Quant Time: Oct 16 01:16:19 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Wed Oct 15 02:12:58 2025
Response via : Initial Calibration




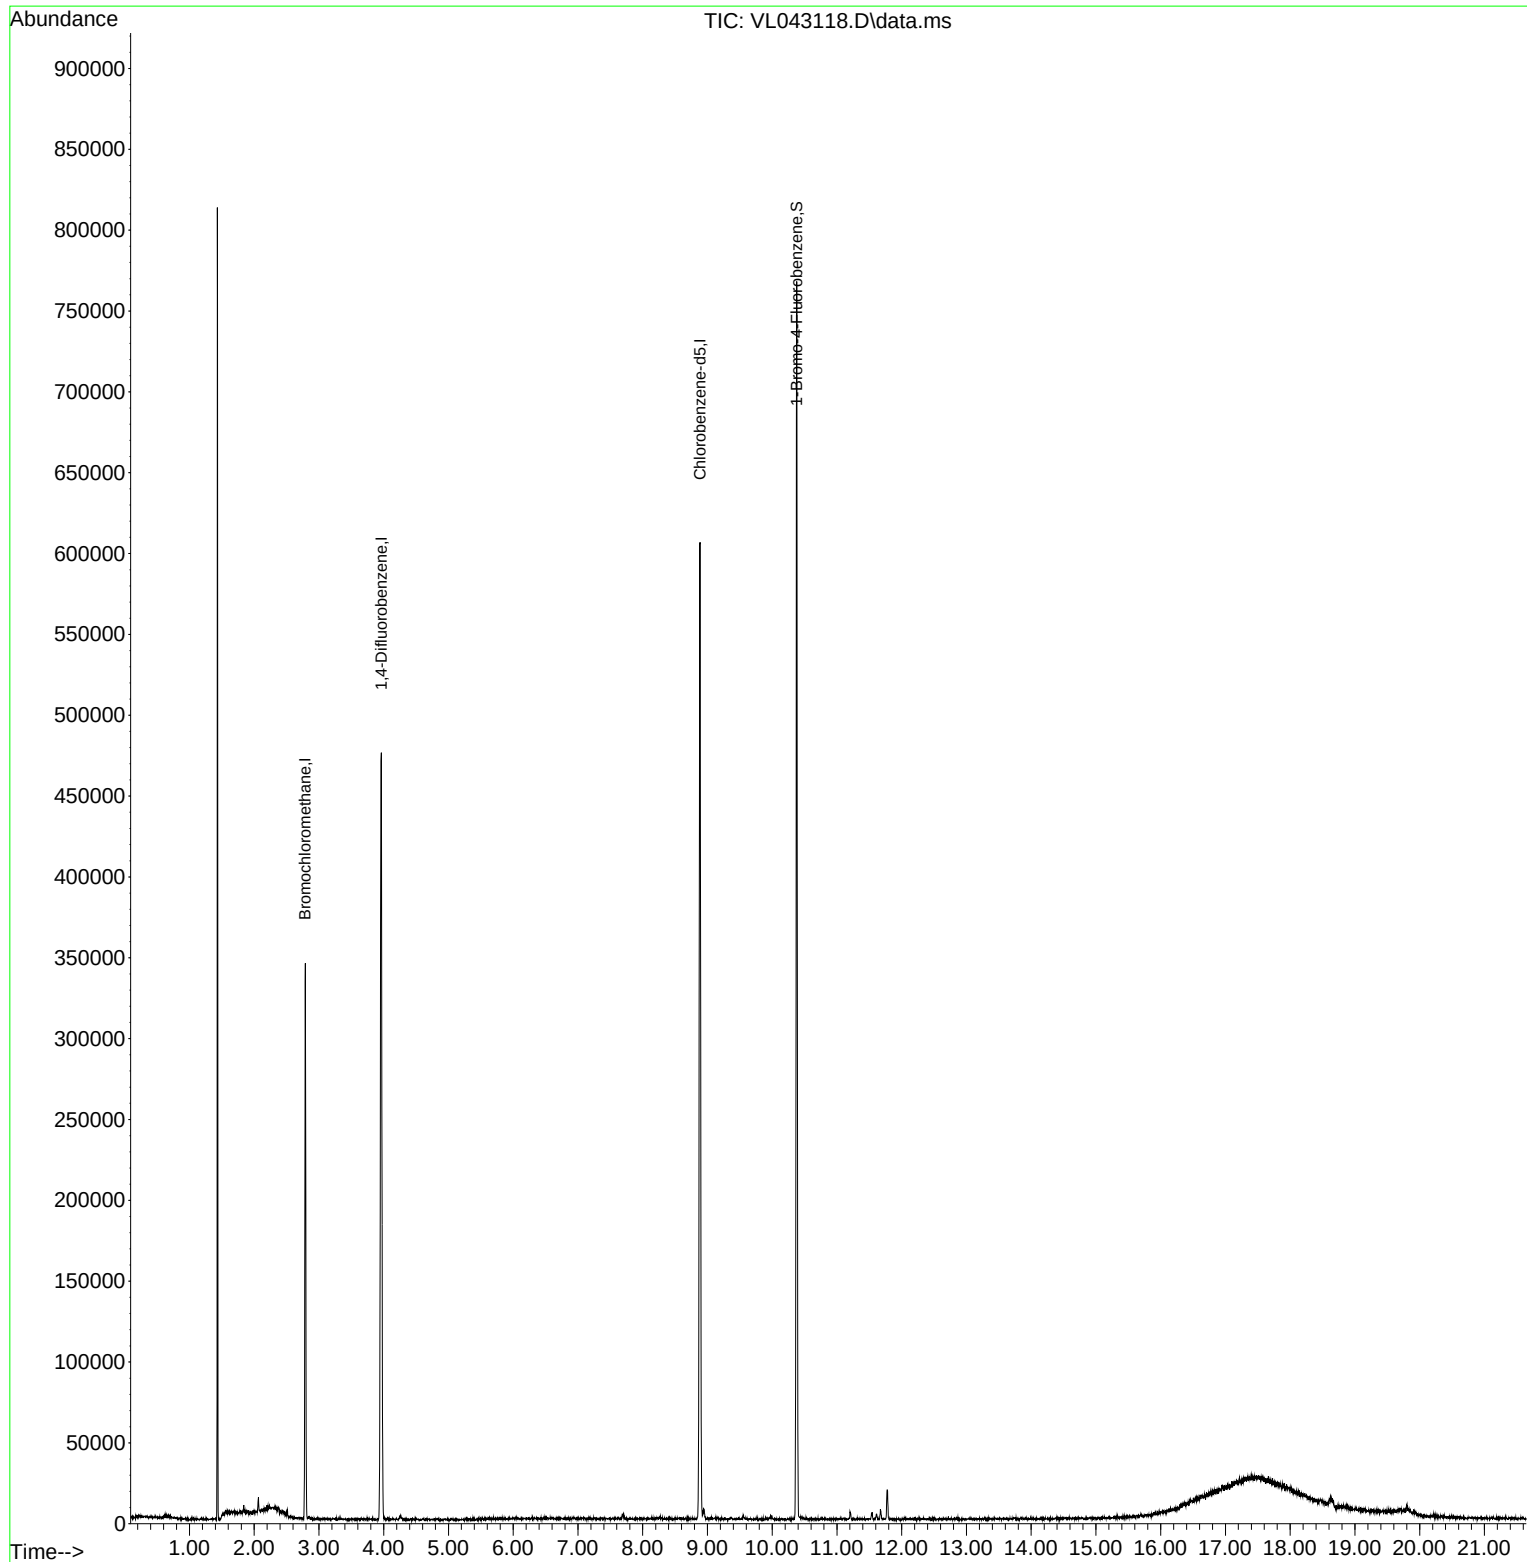


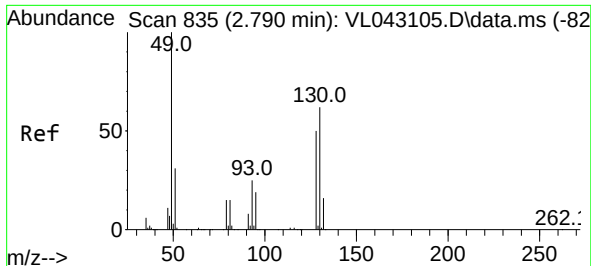

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.787 min Scan# 81
Delta R.T. -0.003 min
Lab File: VL043118.D
Acq: 15 Oct 2025 11:39




Instrument :
MSVOA_L
ClientSampleId :
VIBLK


Tgt Ion: 49 Resp: 90815
Ion Ratio Lower Upper
49 100
128 49.2 24.4 73.4
130 62.5 31.0 93.0

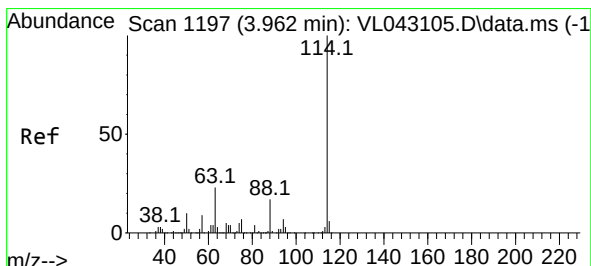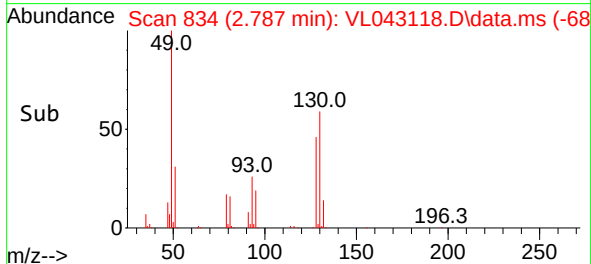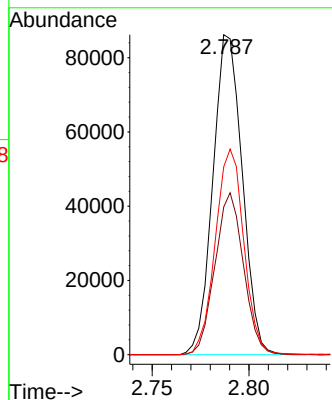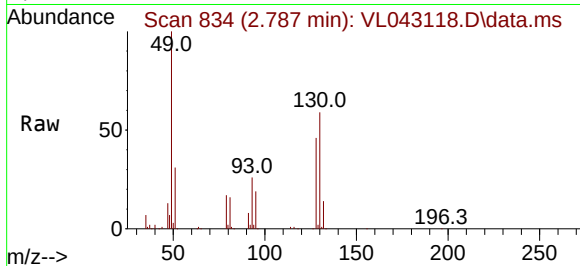

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.962 min Scan# 1197
Delta R.T. -0.000 min
Lab File: VL043118.D
Acq: 15 Oct 2025 11:39

Tgt Ion: 114 Resp: 293345
Ion Ratio Lower Upper
114 100
63 25.0 19.3 28.9
88 17.7 13.9 20.9


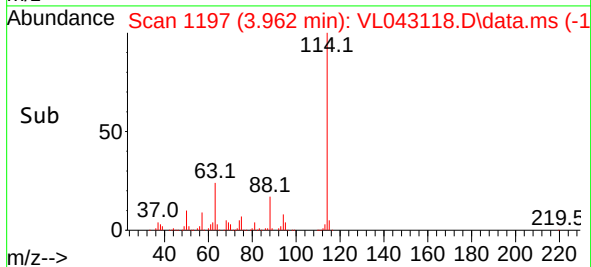
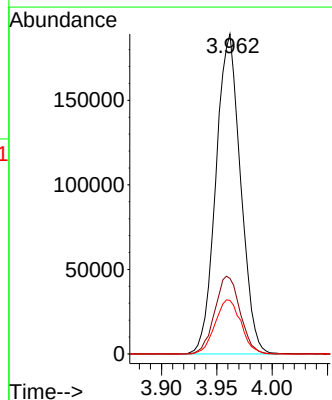
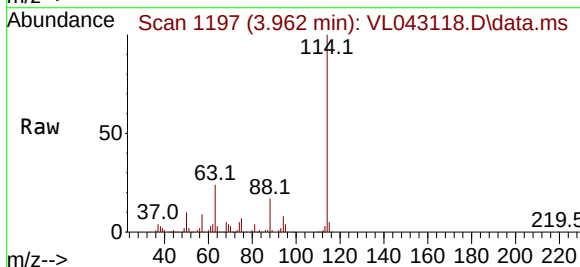


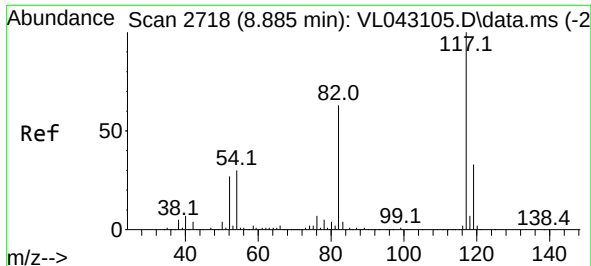

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.885 min Scan# 21
Delta R.T. -0.000 min
Lab File: VL043118.D
Acq: 15 Oct 2025 11:39

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 256803
Ion Ratio Lower Upper
117 100
82 64.8 53.8 80.8
119 31.9 25.4 38.0

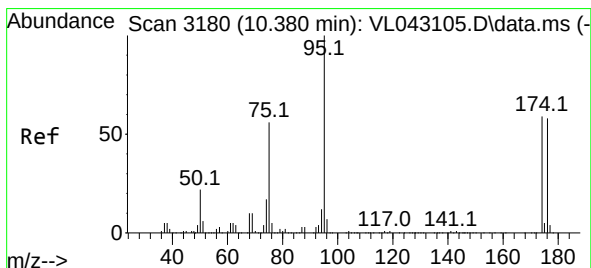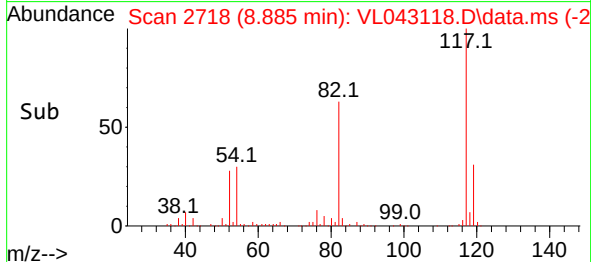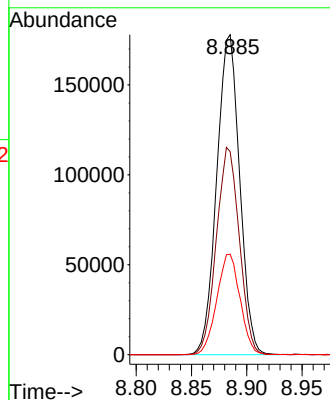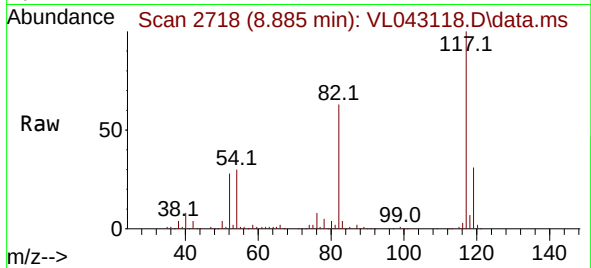

#68
1-Bromo-4-Fluorobenzene
Concen: 10.177 ppbv
RT: 10.377 min Scan# 3179
Delta R.T. -0.003 min
Lab File: VL043118.D
Acq: 15 Oct 2025 11:39

Tgt Ion: 95 Resp: 203144
Ion Ratio Lower Upper
95 100
174 58.6 48.3 72.5
175 4.3 3.8 5.8

