


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL101718\
 Data File : VL032626.D
 Acq On : 17 Oct 2018 2:07
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL101718AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Oct 17 08:55:11 2018
 Last Update : Wed Oct 17 08:55:11 2018

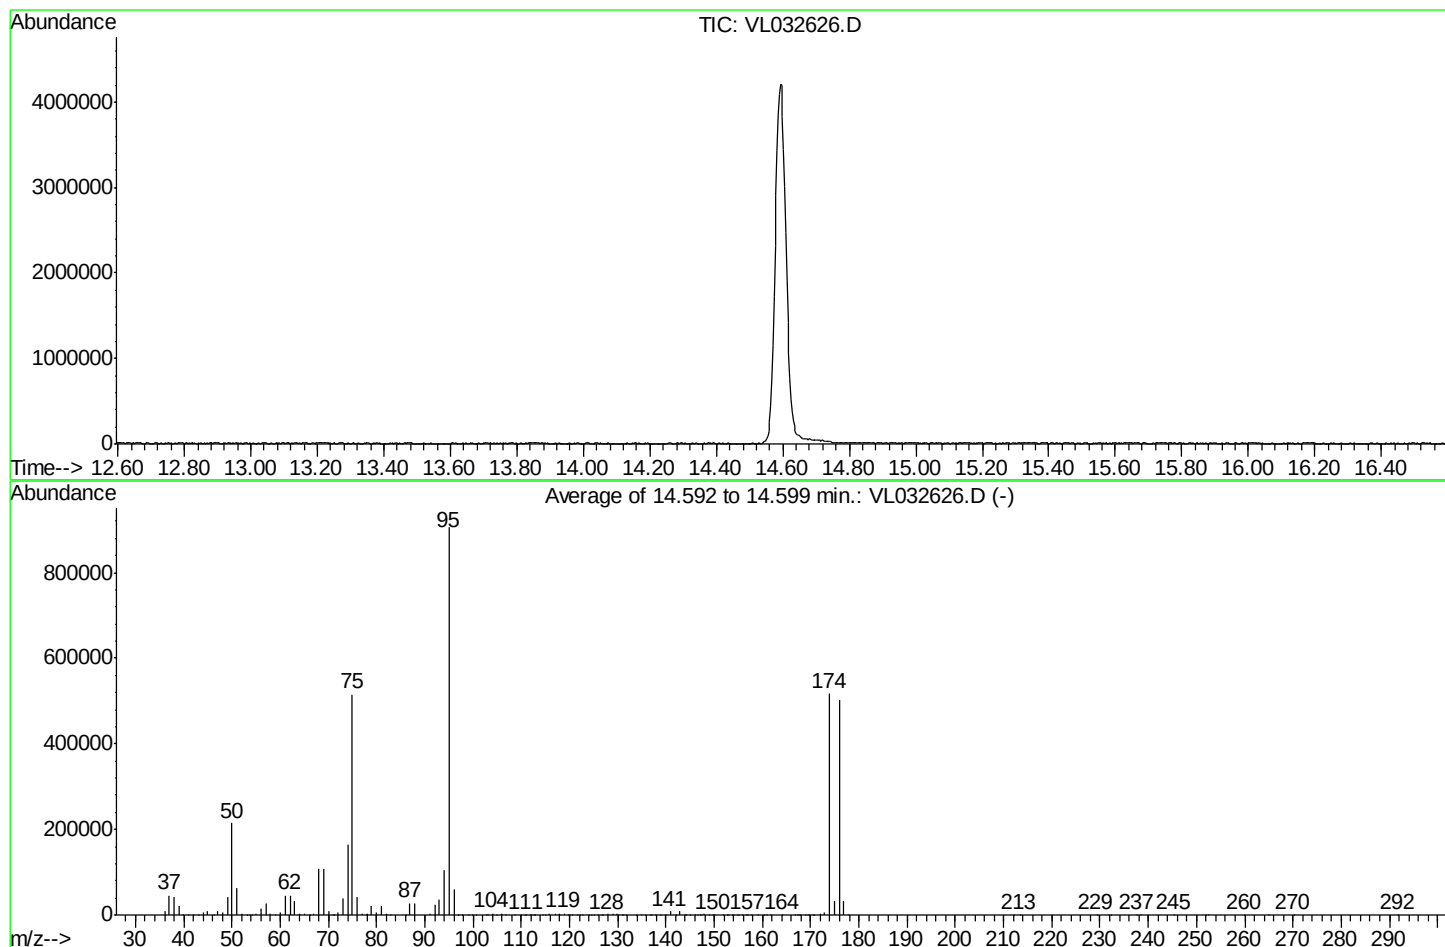

AutoFind: Scans 3625, 3626, 3627; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.7	214528	PASS
75	95	30	66	56.8	514560	PASS
95	95	100	100	100.0	905962	PASS
96	95	5	9	6.7	60864	PASS
173	174	0.00	2	0.9	4777	PASS
174	95	50	120	57.1	517162	PASS
175	174	4	9	6.6	34154	PASS
176	174	93	101	97.4	503466	PASS
177	176	5	9	6.6	33472	PASS