


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL101719\
 Data File : VL034315.D
 Acq On : 17 Oct 2019 12:25
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL101619AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Oct 17 05:12:37 2019
 Last Update : Thu Oct 17 05:12:37 2019

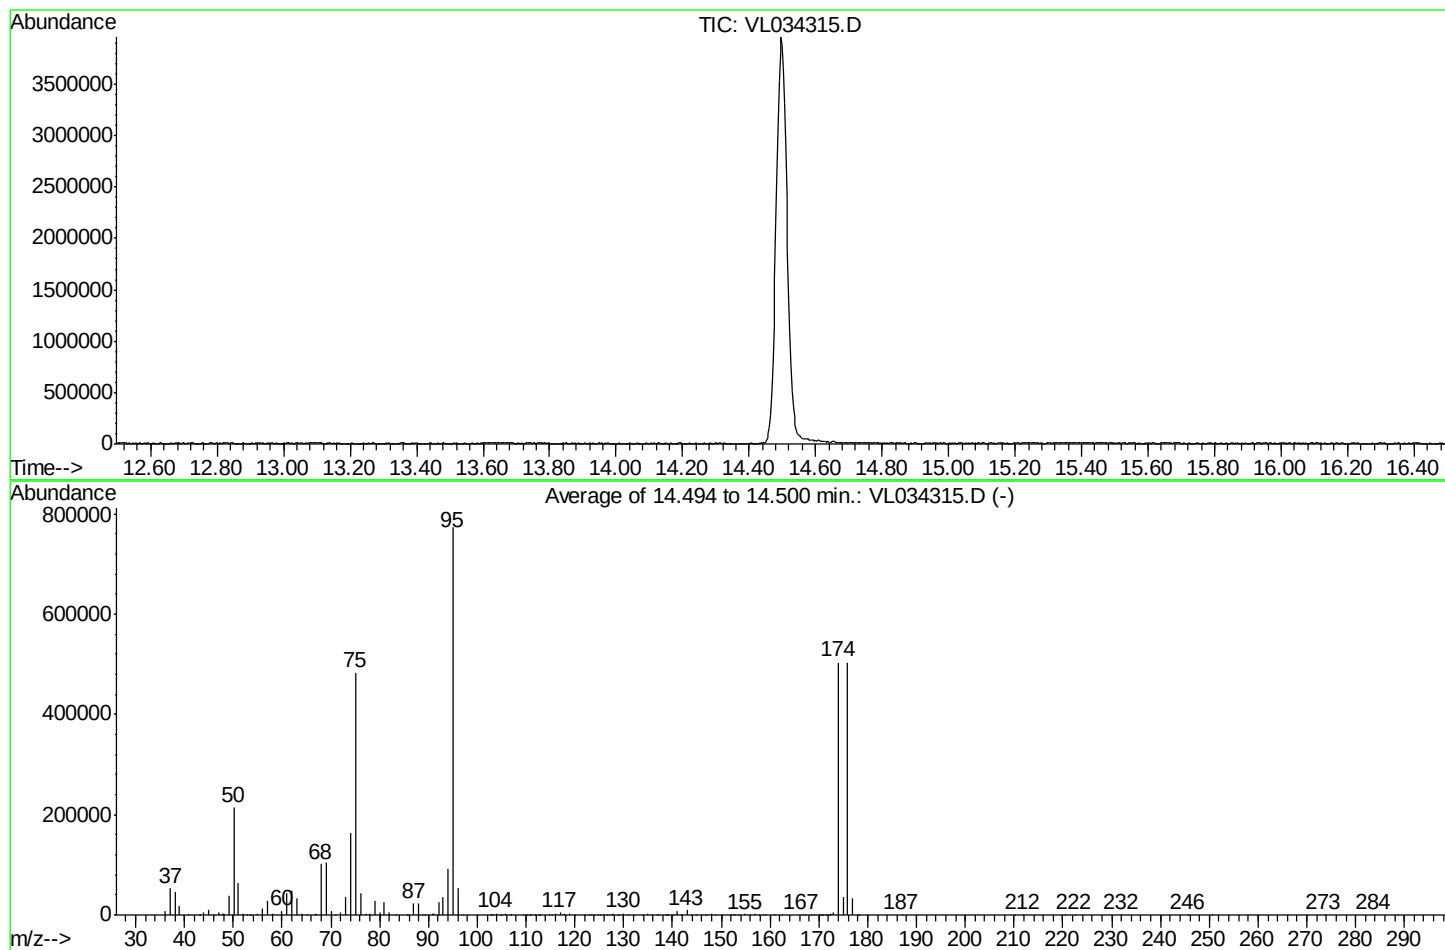

AutoFind: Scans 3641, 3642, 3643; Background Corrected with Scan 3615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.6	213312	PASS
75	95	30	66	62.5	483157	PASS
95	95	100	100	100.0	773376	PASS
96	95	5	9	7.0	54165	PASS
173	174	0.00	2	0.8	4265	PASS
174	95	50	120	65.1	503552	PASS
175	174	4	9	7.1	35693	PASS
176	174	93	101	99.9	503296	PASS
177	176	5	9	6.6	33354	PASS