


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL101818\
Data File : VL032652.D
Acq On : 18 Oct 2018 15:13
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL101818AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Oct 19 01:25:37 2018
Last Update : Fri Oct 19 01:25:37 2018

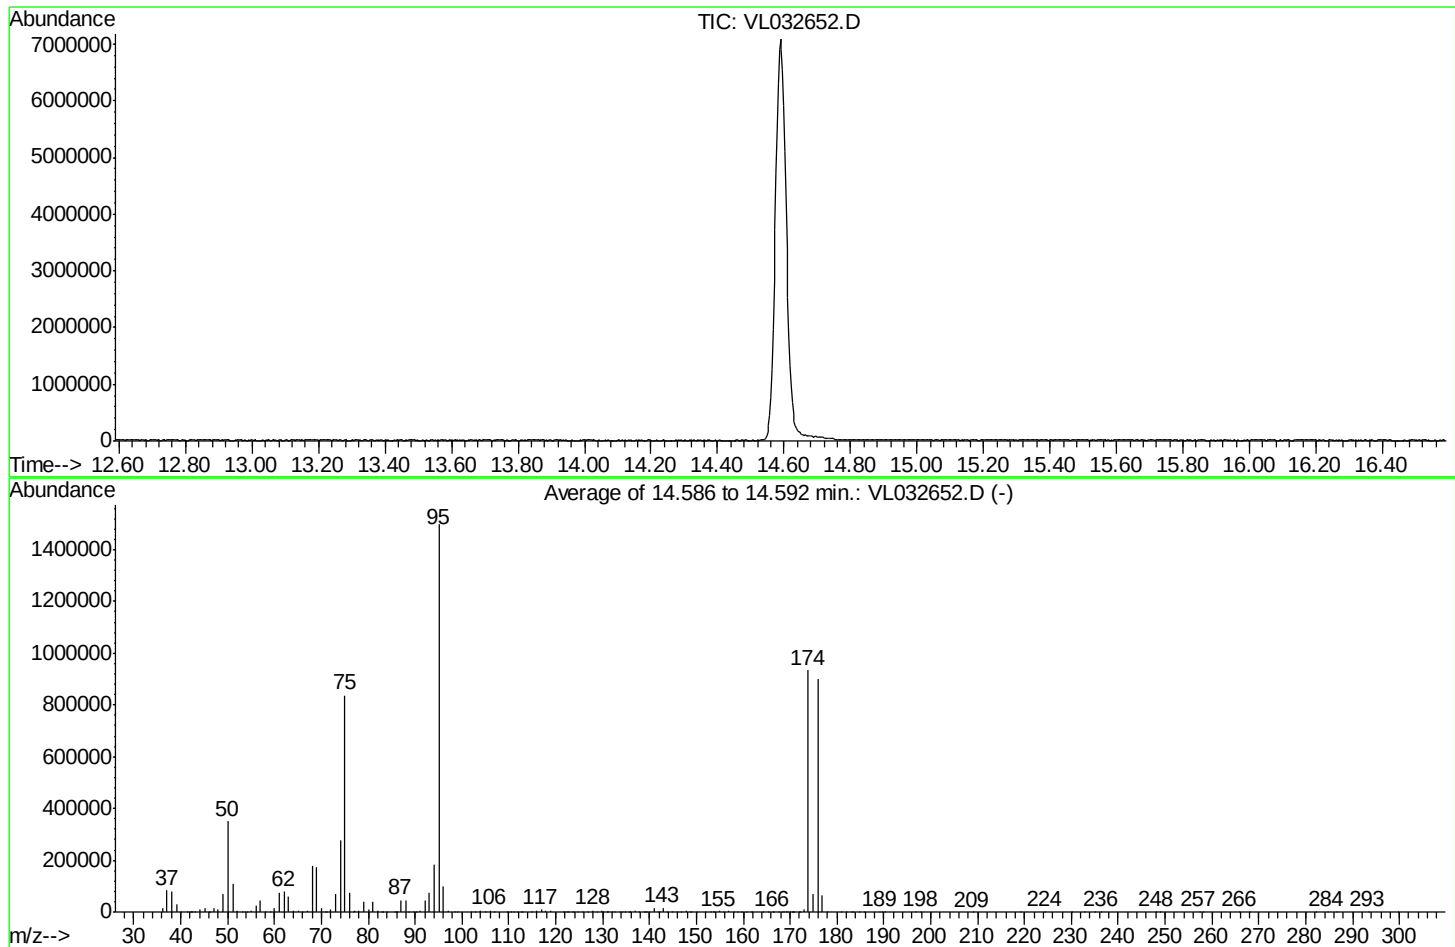

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.4	350144	PASS
75	95	30	66	55.9	836800	PASS
95	95	100	100	100.0	1497941	PASS
96	95	5	9	6.5	97557	PASS
173	174	0.00	2	0.9	8021	PASS
174	95	50	120	62.4	934592	PASS
175	174	4	9	7.6	70976	PASS
176	174	93	101	96.4	901269	PASS
177	176	5	9	6.9	62378	PASS