


Data Path : W:\HPCHEM1\MSVOA L\Data\VL102015\
Data File : VL026205.D
Acq On : 20 Oct 2015 8:37
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL102015AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Oct 21 01:20:55 2015
Last Update : Wed Oct 21 01:20:55 2015

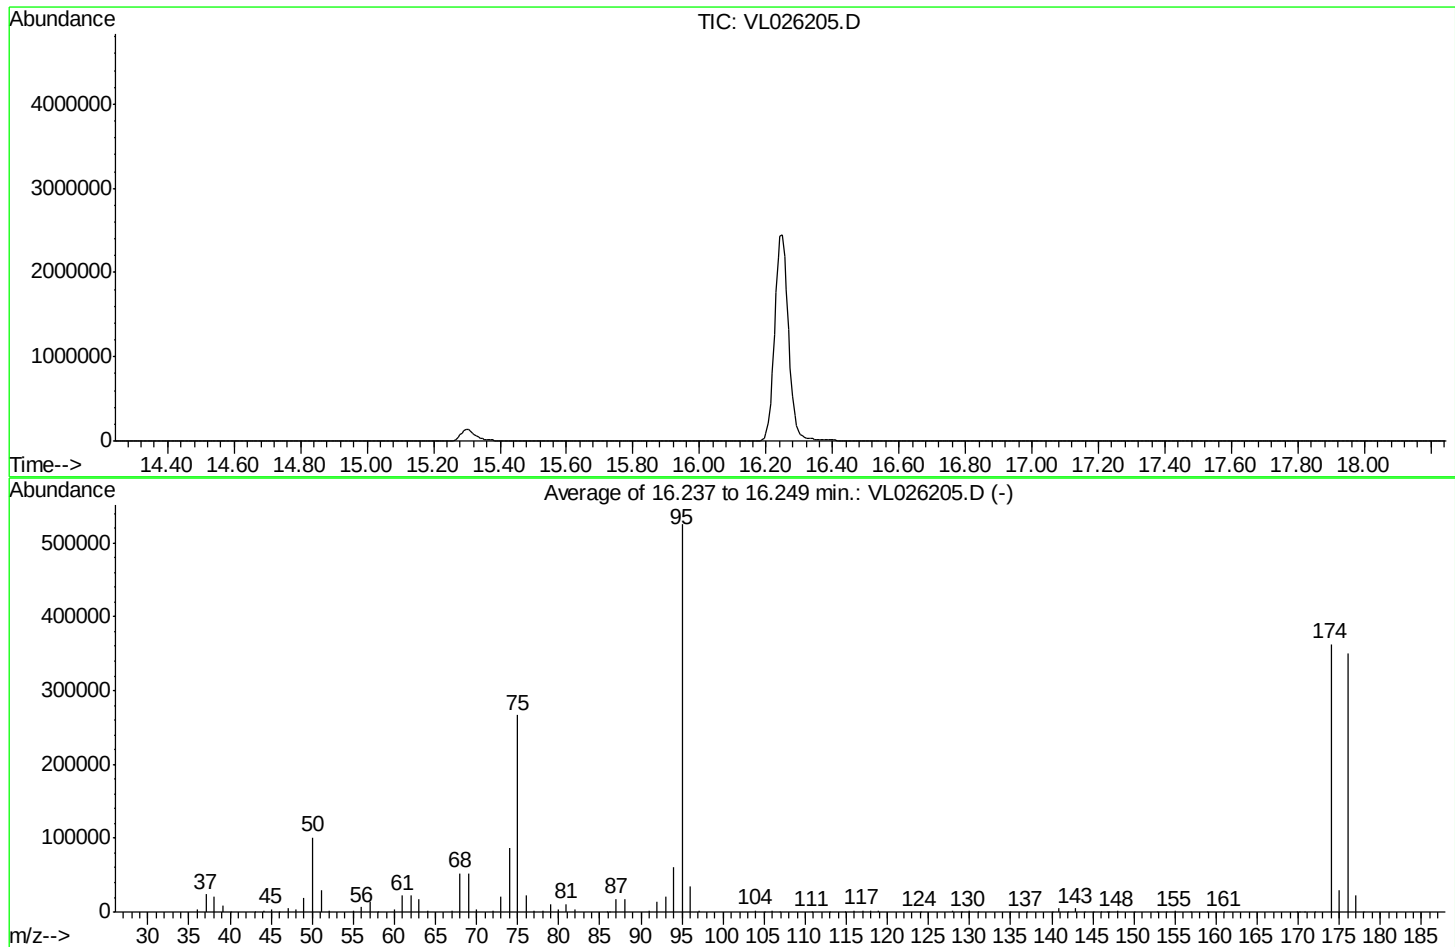

AutoFind: Scans 2157, 2158, 2159; Background Corrected with Scan 2142

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	19.2	100994	PASS
75	95	30	66	50.7	266389	PASS
95	95	100	100	100.0	525376	PASS
96	95	5	9	6.5	34312	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.1	363050	PASS
175	174	4	9	8.3	30069	PASS
176	174	93	101	96.6	350613	PASS
177	176	5	9	6.6	23176	PASS