


Data Path : W:\HPCHEM1\MSVOA L\DATA\VL102115\
 Data File : VL026232.D
 Acq On : 21 Oct 2015 8:53
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL102015AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Oct 21 01:20:55 2015
 Last Update : Wed Oct 21 01:20:55 2015

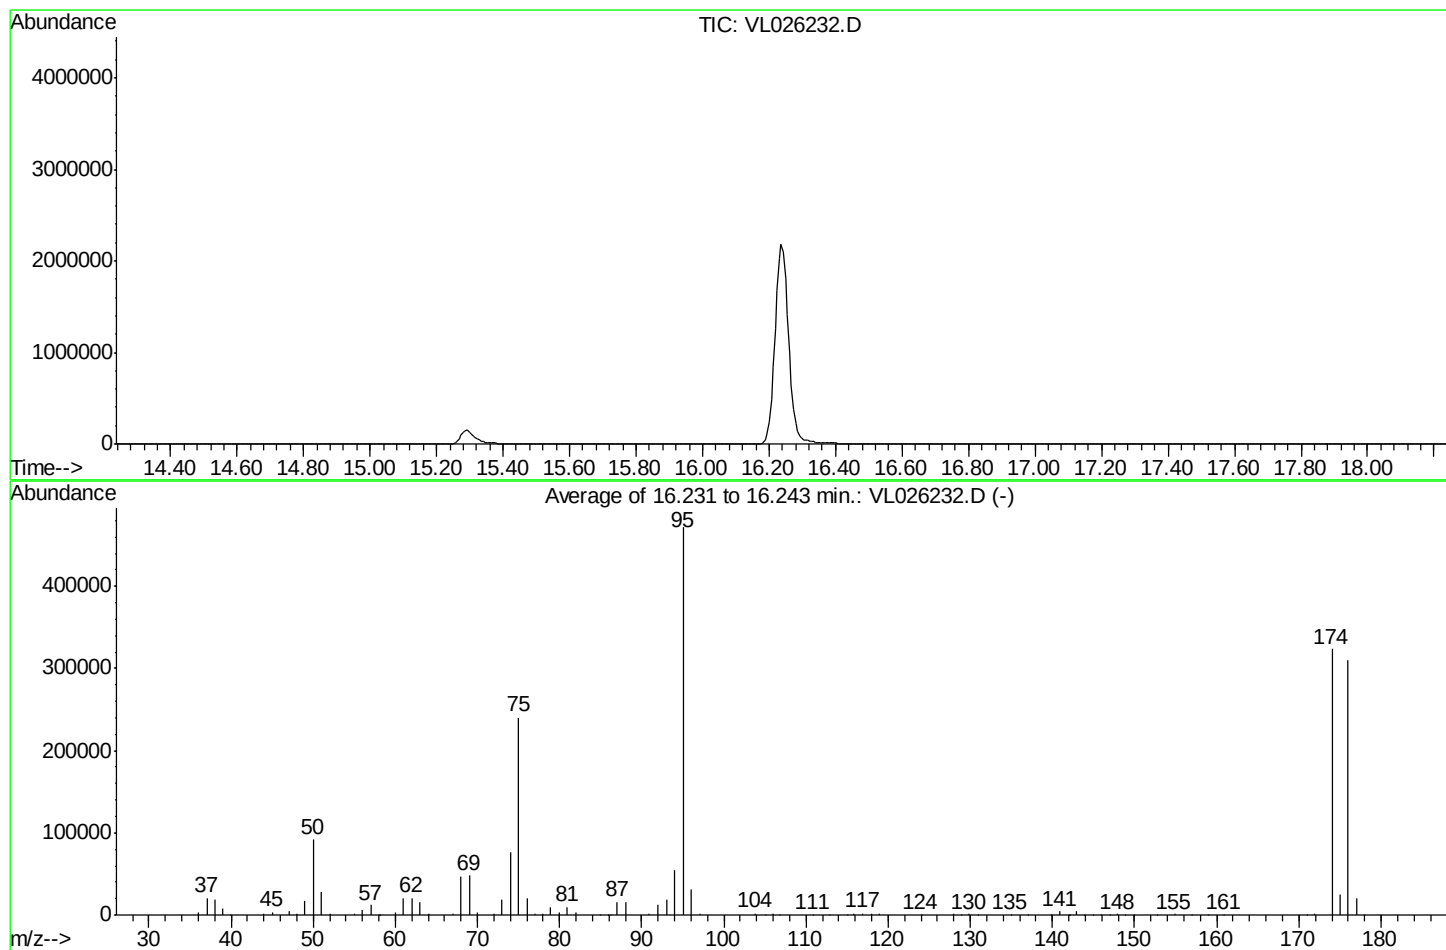

AutoFind: Scans 2156, 2157, 2158; Background Corrected with Scan 2142

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	19.4	91488	PASS
75	95	30	66	50.9	239978	PASS
95	95	100	100	100.0	471701	PASS
96	95	5	9	6.5	30440	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.6	323733	PASS
175	174	4	9	7.6	24730	PASS
176	174	93	101	95.6	309525	PASS
177	176	5	9	6.6	20440	PASS