
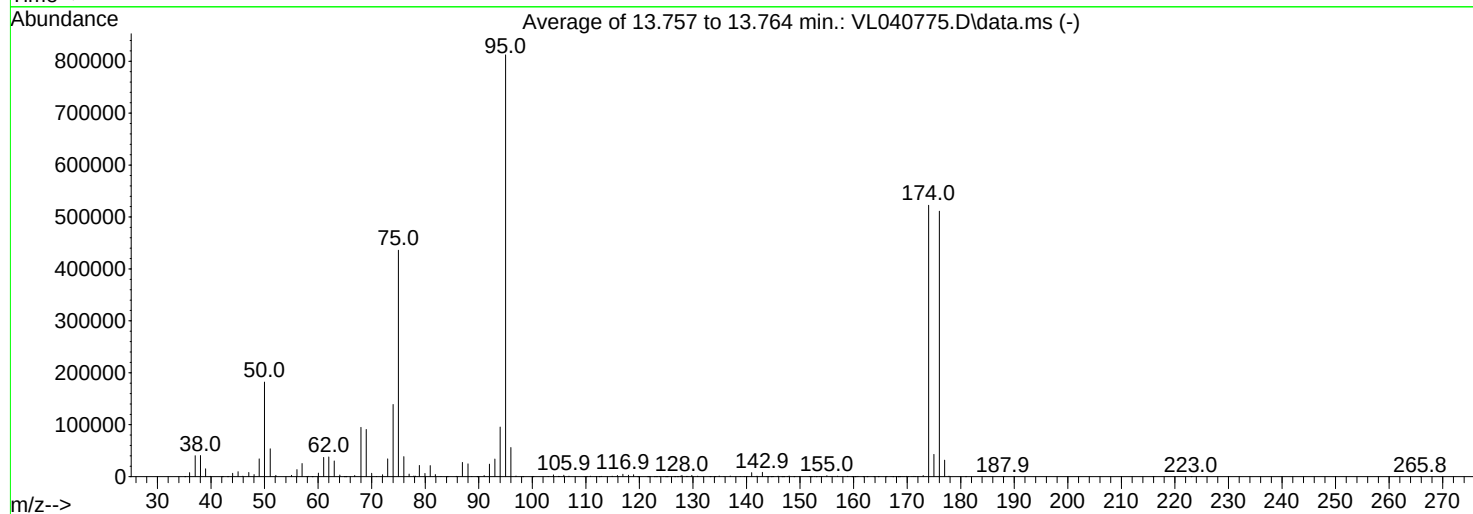


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL102323\
Data File : VL040775.D
Acq On : 23 Oct 2023 12:11
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101123AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Oct 12 00:21:08 2023

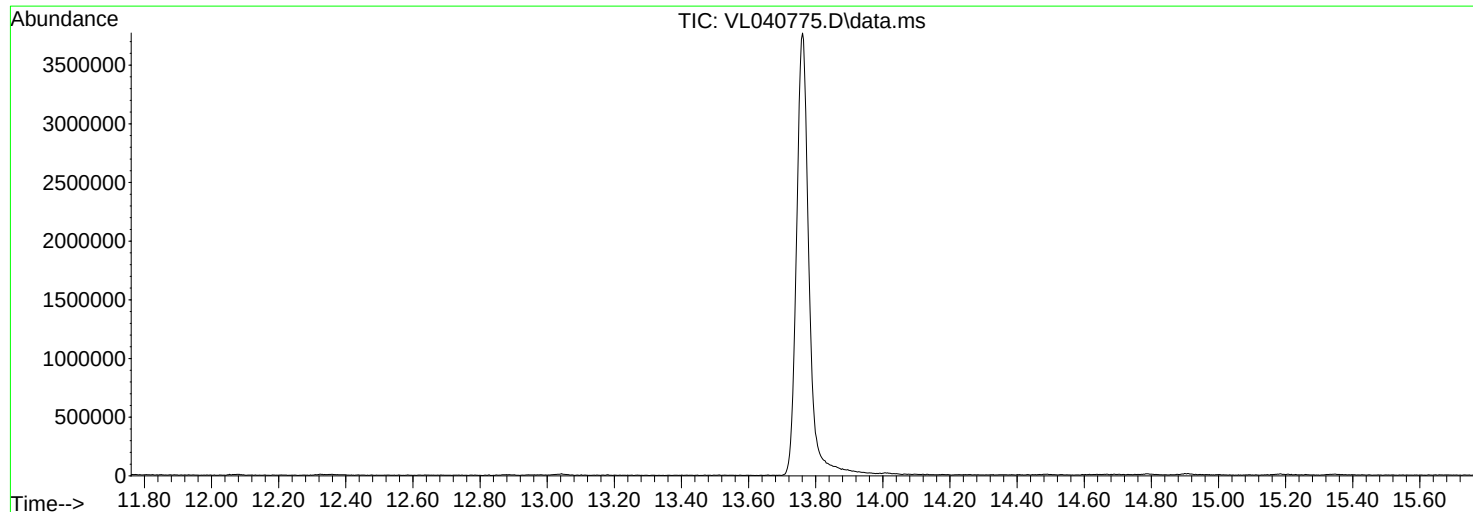

AutoFind: Scans 3469, 3470, 3471; Background Corrected with Scan 3444

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	22.4	182016	PASS
75	95	30	66	53.7	435989	PASS
95	95	100	100	100.0	812288	PASS
96	95	5	9	6.9	55947	PASS
173	174	0.00	2	0.4	2213	PASS
174	95	50	120	64.4	522709	PASS
175	174	4	9	8.2	42723	PASS
176	174	93	101	97.8	511253	PASS
177	176	5	9	6.2	31627	PASS

Average of 13.757 to 13.764 min.: VL040775.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	180	47.05	7979	58.90	79	70.00	6654
36.00	7690	48.05	4181	60.05	6806	70.90	401
37.05	40488	49.00	34293	61.05	37091	72.05	369
38.05	40773	50.00	182016	62.00	37899	73.00	3431
39.00	15103	51.05	53701	63.00	30256	74.00	139029
39.90	603	52.10	2401	64.05	3172	75.00	435989
42.10	81	55.05	2451	64.90	101	76.00	38637
43.10	94	56.05	13472	65.20	59	77.00	4915
44.05	6454	57.00	25328	66.85	2229	77.90	1362
45.05	9616	57.90	221	68.00	94811	78.20	808
45.95	853	58.15	619	69.00	91048	78.90	21624

Average of 13.757 to 13.764 min.: VL040775.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	6106	91.00	2281	104.90	752	115.90	2176
80.95	21243	92.00	23904	105.10	366	116.90	4753
81.90	4024	93.00	33835	105.90	2791	117.95	2843
82.95	420	94.00	95589	106.85	847	118.90	3644
84.10	159	95.00	812288	109.70	362	119.70	94
85.80	489	96.00	55947	110.10	77	121.55	133
86.10	377	96.95	1281	110.85	949	121.80	81
86.95	27307	98.20	84	111.95	372	122.80	156
88.00	24757	100.10	53	112.50	135	123.20	160
88.70	380	102.95	388	112.95	675	123.75	275
89.70	67	103.95	3283	114.90	883	124.55	244

Average of 13.757 to 13.764 min.: VL040775.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.90	172	133.20	64	143.80	298	148.85	186
125.20	171	134.05	190	144.00	143	150.00	776
126.60	91	134.90	1281	144.60	167	151.75	224
127.10	81	135.80	196	144.90	331	151.90	77
127.70	872	136.95	1125	145.05	455	152.10	104
127.95	2430	138.85	330	145.90	1078	152.70	408
128.80	628	139.60	366	146.60	85	153.00	163
129.05	772	140.10	232	146.90	120	153.70	214
129.80	2412	140.95	7806	147.05	314	154.00	240
130.90	990	141.95	1101	147.70	468	155.00	1890
131.90	246	142.95	8281	147.95	1269	155.75	421

Average of 13.757 to 13.764 min.: VL040775.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.00	911	167.30	183	172.00	329	265.80	76
158.90	794	167.95	229	173.00	2213		
159.70	70	168.30	133	174.00	522709		
160.30	82	168.60	82	175.00	42723		
160.80	795	169.05	425	176.00	511253		
161.80	75	169.40	235	177.00	31627		
162.50	68	169.85	552	177.80	1076		
163.80	131	170.20	209	180.90	71		
164.60	111	170.90	316	187.90	84		
166.05	118	171.25	591	215.90	59		
167.00	248	171.50	260	223.00	71		