


Data Path : \\74.0.250.170\terastorage\voasrv\HPCHEM1\MSVOA_L\Data\VL102419\
Data File : VL034341.D
Acq On : 24 Oct 2019 9:12
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL101619AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Oct 17 05:12:37 2019
Last Update : Thu Oct 17 05:12:37 2019

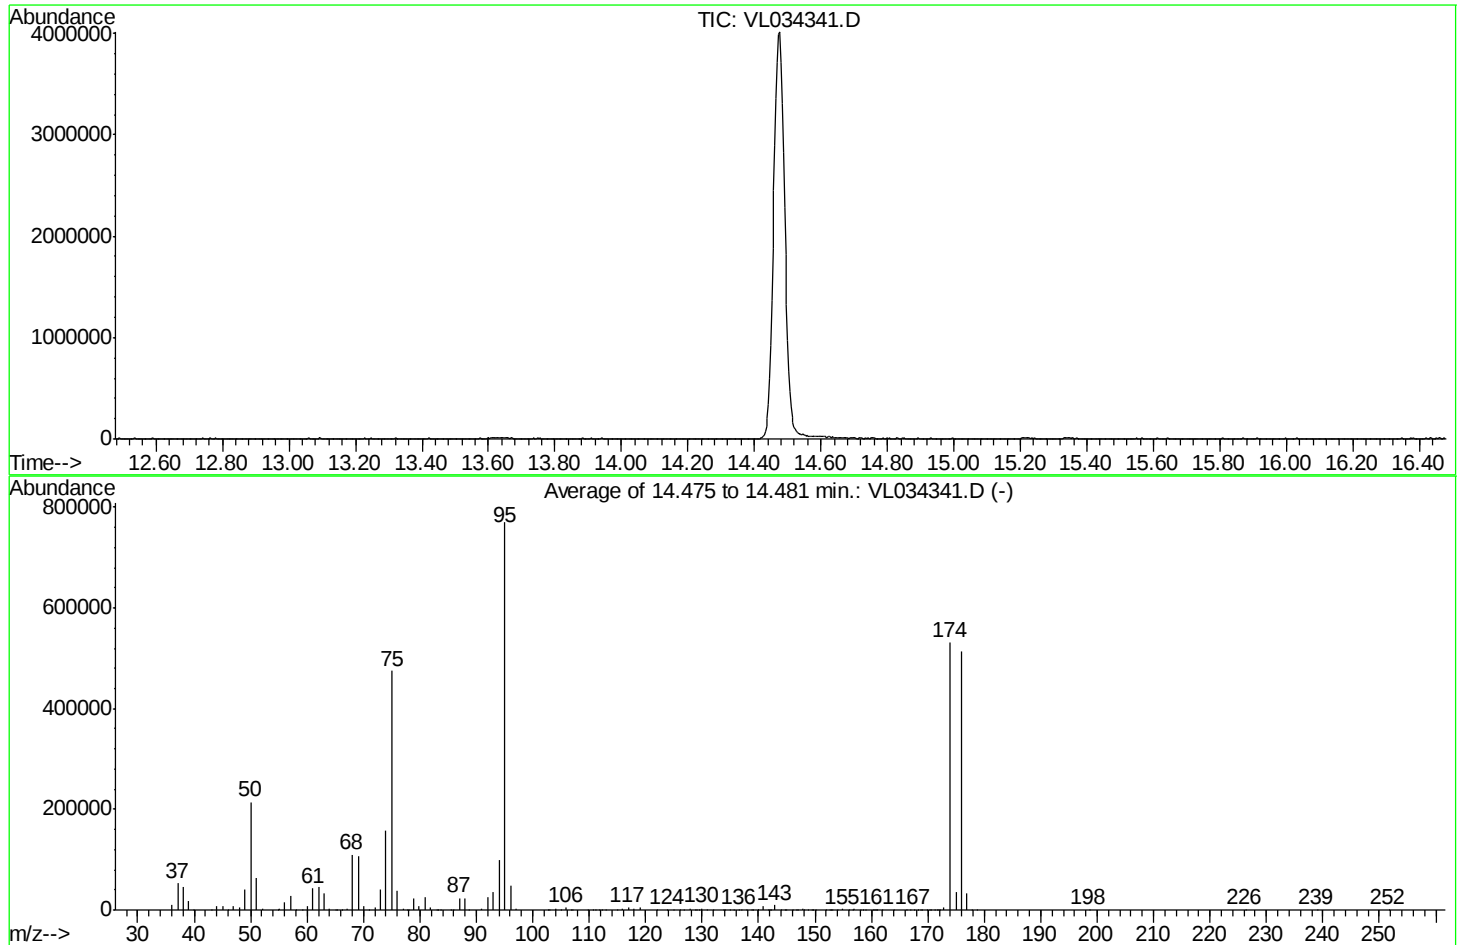

AutoFind: Scans 3635, 3636, 3637; Background Corrected with Scan 3609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.8	213824	PASS
75	95	30	66	61.6	474581	PASS
95	95	100	100	100.0	770112	PASS
96	95	5	9	6.4	49634	PASS
173	174	0.00	2	0.9	4722	PASS
174	95	50	120	68.9	530474	PASS
175	174	4	9	6.8	35981	PASS
176	174	93	101	96.9	514240	PASS
177	176	5	9	6.2	32138	PASS