

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL102422\
 Data File : VL039770.D
 Acq On : 24 Oct 2022 23:33
 Operator : SY/AP
 Sample : N5227-01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 3

Min Area: 3 % of largest Peak

Start Thrs: 0.001

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 0

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL102422AIR.M

Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

Signal : TIC: VL039770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.726	32	38	43	rBV3	80009	89629	1.21%	0.241%
2	2.890	80	89	106	rBV2	495463	756224	10.18%	2.033%
3	3.028	125	132	142	rBV2	262023	326404	4.39%	0.877%
4	3.256	194	203	213	rBV	130505	263275	3.54%	0.708%
5	3.484	264	274	277	rBV	746929	891595	12.00%	2.397%
6	3.504	277	280	298	rVV	702299	1144032	15.40%	3.075%
7	3.594	298	308	316	rVV3	125335	283484	3.82%	0.762%
8	3.697	332	340	347	rBV2	65021	79791	1.07%	0.214%
9	3.748	348	356	368	rVB2	278571	388430	5.23%	1.044%
10	3.819	368	378	394	rVB7	78460	154770	2.08%	0.416%
11	3.912	397	407	410	rBV6	59518	81557	1.10%	0.219%
12	3.947	410	418	433	rVB3	511234	907060	12.21%	2.438%
13	4.619	615	627	634	rBV4	89455	168685	2.27%	0.453%
14	4.668	634	642	654	rVB2	174846	319867	4.31%	0.860%
15	4.918	707	720	730	rBV2	99960	180643	2.43%	0.486%
16	5.198	791	807	828	rBV2	1871509	4348281	58.53%	11.689%
17	5.269	828	829	849	rVB8	77549	151885	2.04%	0.408%
18	5.545	908	915	928	rBV6	59510	123411	1.66%	0.332%
19	5.822	989	1001	1027	rVB5	130957	339444	4.57%	0.913%
20	6.323	1146	1157	1162	rBV9	46462	85522	1.15%	0.230%
21	6.375	1164	1173	1184	rVB3	92150	187447	2.52%	0.504%
22	6.606	1230	1245	1247	rBV5	83358	133456	1.80%	0.359%
23	6.655	1247	1260	1279	rVV	3046679	6215563	83.67%	16.709%
24	6.725	1279	1282	1296	rVV5	136492	284120	3.82%	0.764%
25	6.957	1343	1354	1364	rBV5	65836	131722	1.77%	0.354%
26	7.327	1451	1469	1484	rVB3	159918	383690	5.16%	1.031%
27	7.577	1533	1547	1548	rBV2	101611	109987	1.48%	0.296%
28	7.584	1548	1549	1558	rVB5	78145	77345	1.04%	0.208%
29	8.243	1741	1754	1768	rBV5	81743	175187	2.36%	0.471%
30	9.217	2039	2057	2075	rBV2	346311	764762	10.29%	2.056%
31	9.478	2125	2138	2144	rBV6	39294	81375	1.10%	0.219%
32	10.487	2438	2452	2469	rBV3	96994	227087	3.06%	0.610%
33	11.462	2735	2755	2781	rBV2	3009670	7242389	97.49%	19.469%
34	12.082	2936	2948	2957	rBV6	47298	104532	1.41%	0.281%
35	12.339	3016	3028	3052	rBV4	121331	421577	5.67%	1.133%
36	13.053	3236	3250	3252	rBV4	62289	96498	1.30%	0.259%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL102422\
Data File : VL039770.D
Acq On : 24 Oct 2022 23:33
Operator : SY/AP
Sample : N5227-01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 3

Min Area: 3 % of largest Peak

Start Thrs: 0.001

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 0

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL102422AIR.M

Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

37	13.526	3380	3397	3412	rBV3	253272	578844	7.79%	1.556%
38	13.767	3454	3472	3496	rBV4	2964039	7428842	100.00%	19.971%
39	13.847	3496	3497	3507	rVB8	73825	93444	1.26%	0.251%
40	15.124	3881	3894	3901	rBV2	48958	99391	1.34%	0.267%
41	16.101	4180	4198	4215	rBV5	82435	238988	3.22%	0.642%
42	16.365	4263	4280	4281	rBV6	54768	83682	1.13%	0.225%
43	16.375	4281	4283	4296	rVB5	69523	97056	1.31%	0.261%
44	16.477	4296	4315	4327	rBV5	153828	377015	5.08%	1.014%
45	20.792	5632	5657	5670	rBV2	160999	480839	6.47%	1.293%




Sum of corrected areas: 37198827

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL102422\
Data File : VL039770.D
Acq On : 24 Oct 2022 23:33
Operator : SY/AP
Sample : N5227-01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL102422AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

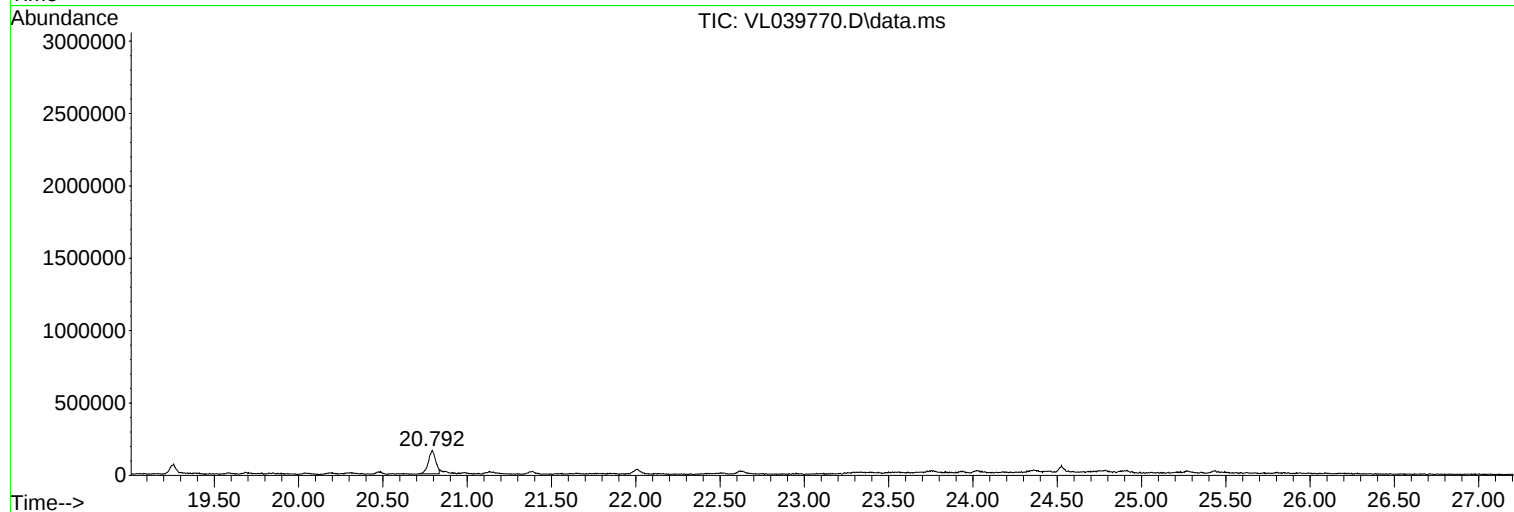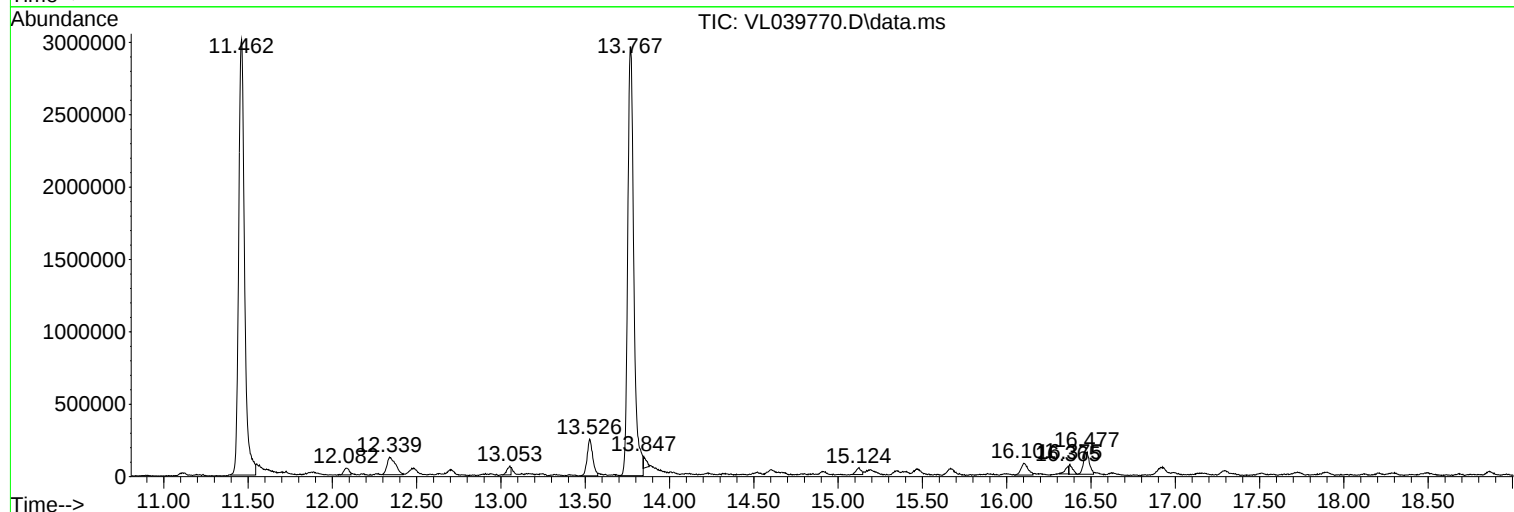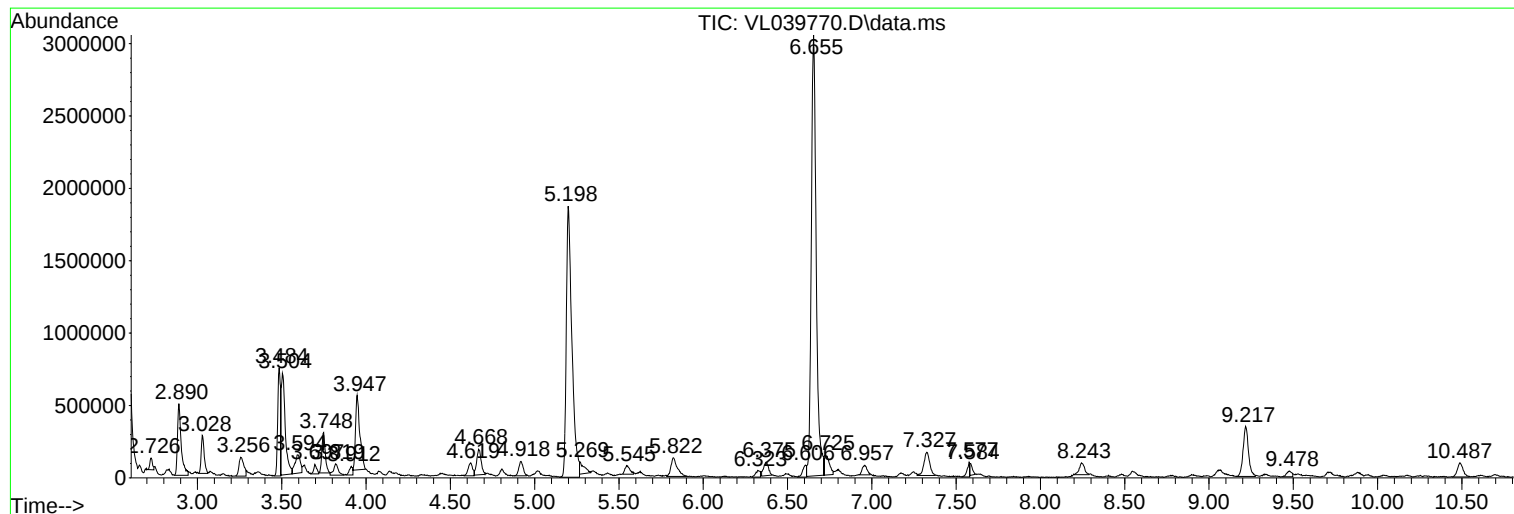

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL102422\
Data File : VL039770.D
Acq On : 24 Oct 2022 23:33
Operator : SY/AP
Sample : N5227-01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL102422AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL102422\
Data File : VL039770.D
Acq On : 24 Oct 2022 23:33
Operator : SY/AP
Sample : N5227-01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL102422AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc