
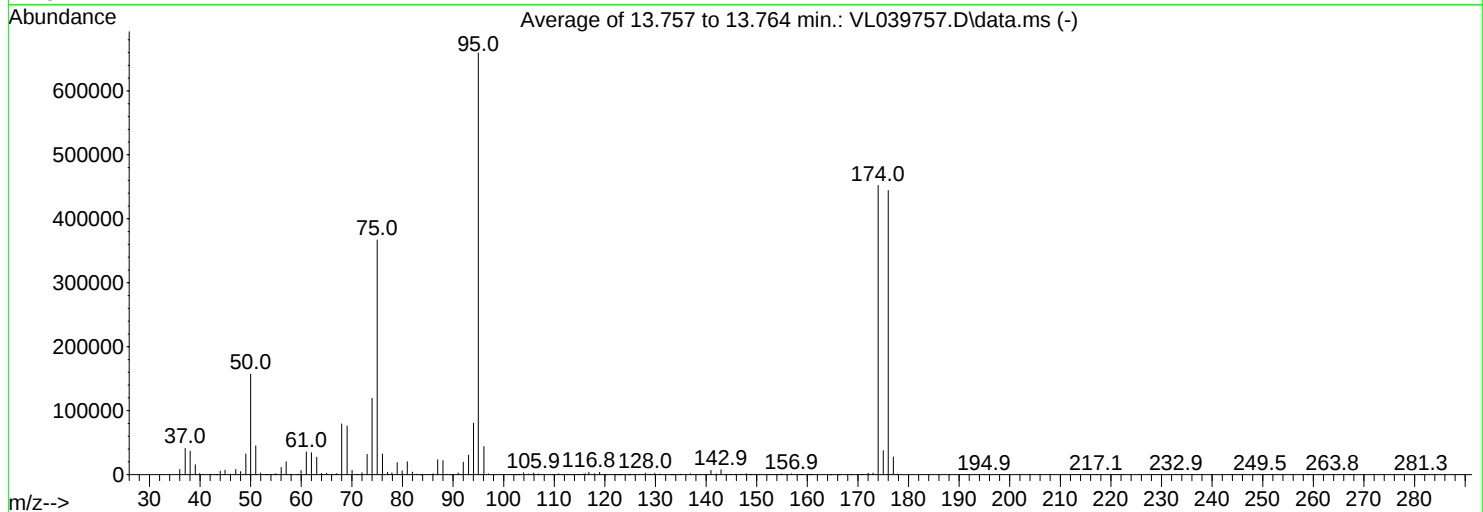


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL102422\
Data File : VL039757.D
Acq On : 24 Oct 2022 10:17
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL102422AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Mon Oct 24 20:00:55 2022

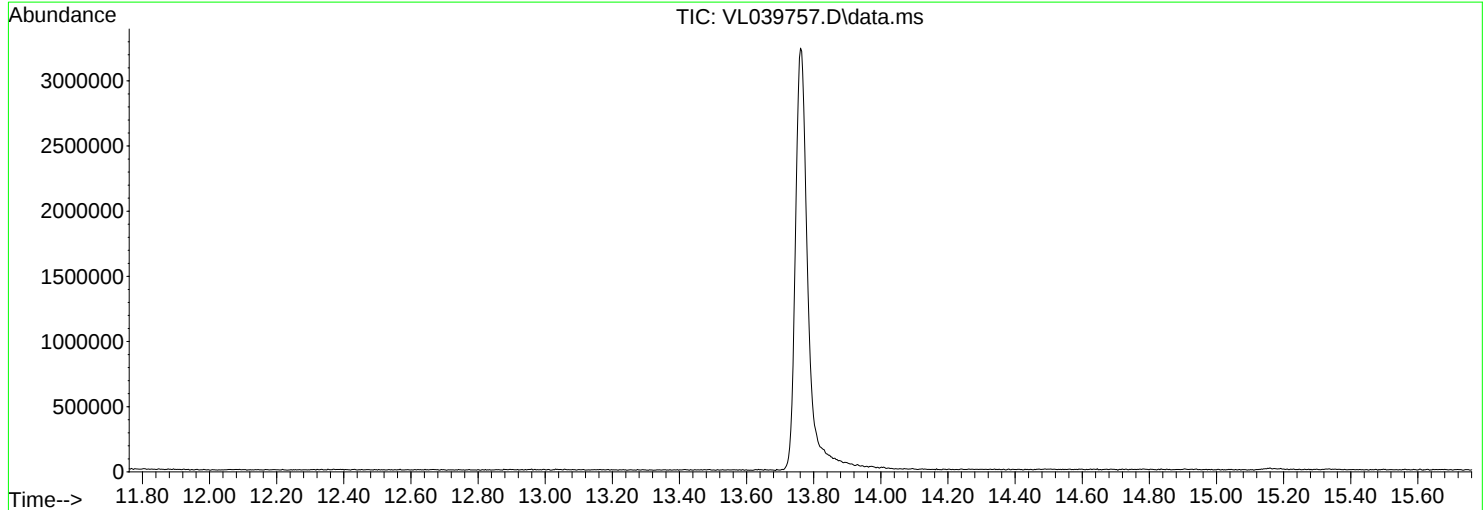

AutoFind: Scans 3469, 3470, 3471; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	157035	PASS
75	95	30	66	55.7	367125	PASS
95	95	100	100	100.0	659520	PASS
96	95	5	9	6.7	44152	PASS
173	174	0.00	2	0.5	2433	PASS
174	95	50	120	68.5	452053	PASS
175	174	4	9	8.3	37472	PASS
176	174	93	101	98.3	444395	PASS
177	176	5	9	6.2	27424	PASS

Average of 13.757 to 13.764 min.: VL039757.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8098	47.05	8036	56.05	11508	66.80	511
37.05	41133	48.00	4678	57.00	20315	67.05	181
38.05	36845	49.05	32365	58.00	718	68.00	7924
39.05	15572	50.00	157035	59.20	109	69.05	7608
39.95	2039	51.00	45107	59.95	6473	70.05	6705
42.00	71	51.95	2550	61.00	35624	71.00	62
42.75	394	52.20	440	62.00	34392	71.80	599
43.20	156	52.95	360	63.05	27277	72.00	3038
44.00	5489	53.20	119	64.00	2002	73.00	31915
44.95	7009	54.80	730	65.00	2394	74.00	119325
46.05	897	55.00	1594	66.10	379	75.00	367125

Average of 13.757 to 13.764 min.: VL039757.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	32347	86.05	1556	97.00	1207	111.70	312
77.05	3800	86.95	23237	98.00	79	111.90	225
77.90	2887	88.00	21928	102.40	73	112.60	278
78.95	18787	88.80	187	103.00	90	113.00	534
79.95	6120	89.70	56	103.95	2956	113.70	58
80.95	20293	91.00	2681	104.85	1088	114.15	260
81.95	4083	92.00	19595	105.90	2485	114.65	633
82.85	698	93.05	30624	106.95	1204	114.90	311
83.50	61	94.05	80613	109.75	245	115.10	170
83.70	60	95.00	659520	110.00	109	115.80	878
83.90	51	96.10	44152	110.90	1258	116.10	1516

Average of 13.757 to 13.764 min.: VL039757.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.85	3862	124.90	80	134.70	320	143.75	192
117.90	1583	125.85	260	134.95	888	144.30	277
118.95	3491	126.90	228	135.90	372	144.95	841
120.05	132	128.00	2434	136.90	1251	145.80	418
121.90	133	128.90	661	138.60	206	145.95	654
122.10	93	129.85	2383	138.85	316	147.00	219
122.70	92	130.90	911	139.80	300	147.90	1434
123.00	128	131.75	333	140.00	219	148.60	175
123.50	220	133.10	95	140.95	6722	148.80	129
124.00	311	133.50	90	142.00	1158	149.10	167
124.70	124	133.80	157	142.95	7886	149.80	458

Average of 13.757 to 13.764 min.: VL039757.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
149.95	413	157.80	171	169.80	76	177.00	27424
150.60	232	158.00	63	170.15	352	177.85	947
151.95	321	158.80	368	170.60	215	194.95	171
152.80	276	158.95	364	170.90	246	217.10	53
153.00	326	160.50	110	171.20	229	232.90	208
153.80	363	160.85	612	172.00	2210	243.90	65
154.20	294	161.10	196	172.20	865	249.50	160
154.70	462	164.60	129	173.00	2433	258.90	74
154.95	1010	166.30	58	174.00	452053	263.80	95
156.10	366	168.60	284	175.00	37472	267.10	58
156.90	1185	168.85	427	176.00	444395	281.30	50