


Data Path : \\74.0.250.170\Terastorage\voasrv\HPCHEM1\MSVOA_L\Data\VL102519\
Data File : VL034358.D
Acq On : 25 Oct 2019 9:35
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL101619AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Oct 17 05:12:37 2019
Last Update : Thu Oct 17 05:12:37 2019

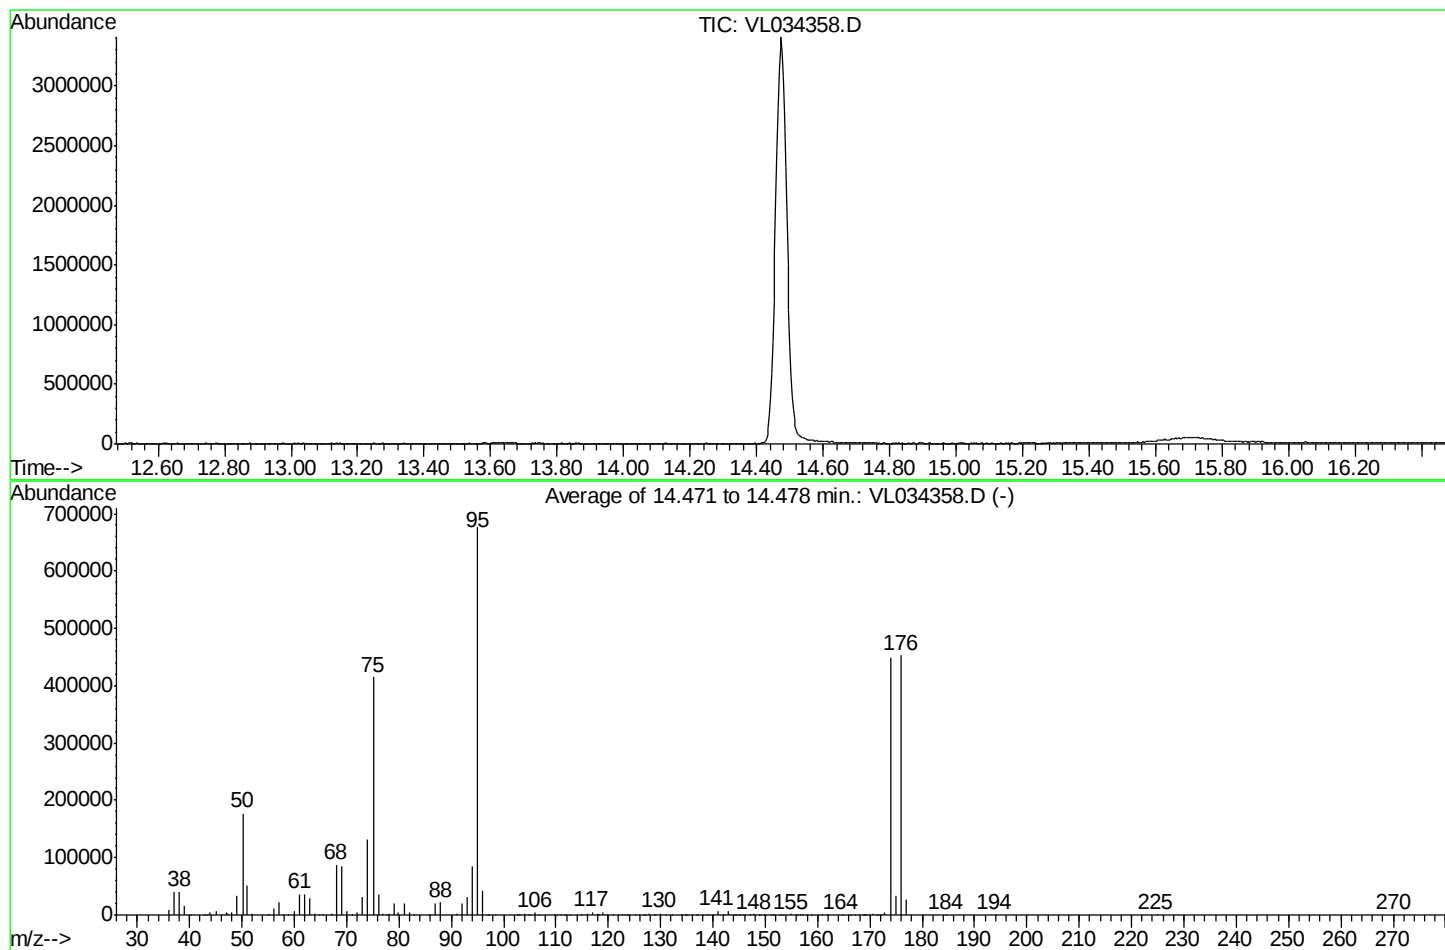

AutoFind: Scans 3634, 3635, 3636; Background Corrected with Scan 3609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.1	176704	PASS
75	95	30	66	61.3	414762	PASS
95	95	100	100	100.0	676224	PASS
96	95	5	9	6.4	43533	PASS
173	174	0.00	2	0.9	4001	PASS
174	95	50	120	66.4	448853	PASS
175	174	4	9	7.4	33410	PASS
176	174	93	101	101.0	453226	PASS
177	176	5	9	6.1	27757	PASS