


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL102522\
Data File : VL039786.D
Acq On : 25 Oct 2022 10:49
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL102422AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Mon Oct 24 20:00:55 2022

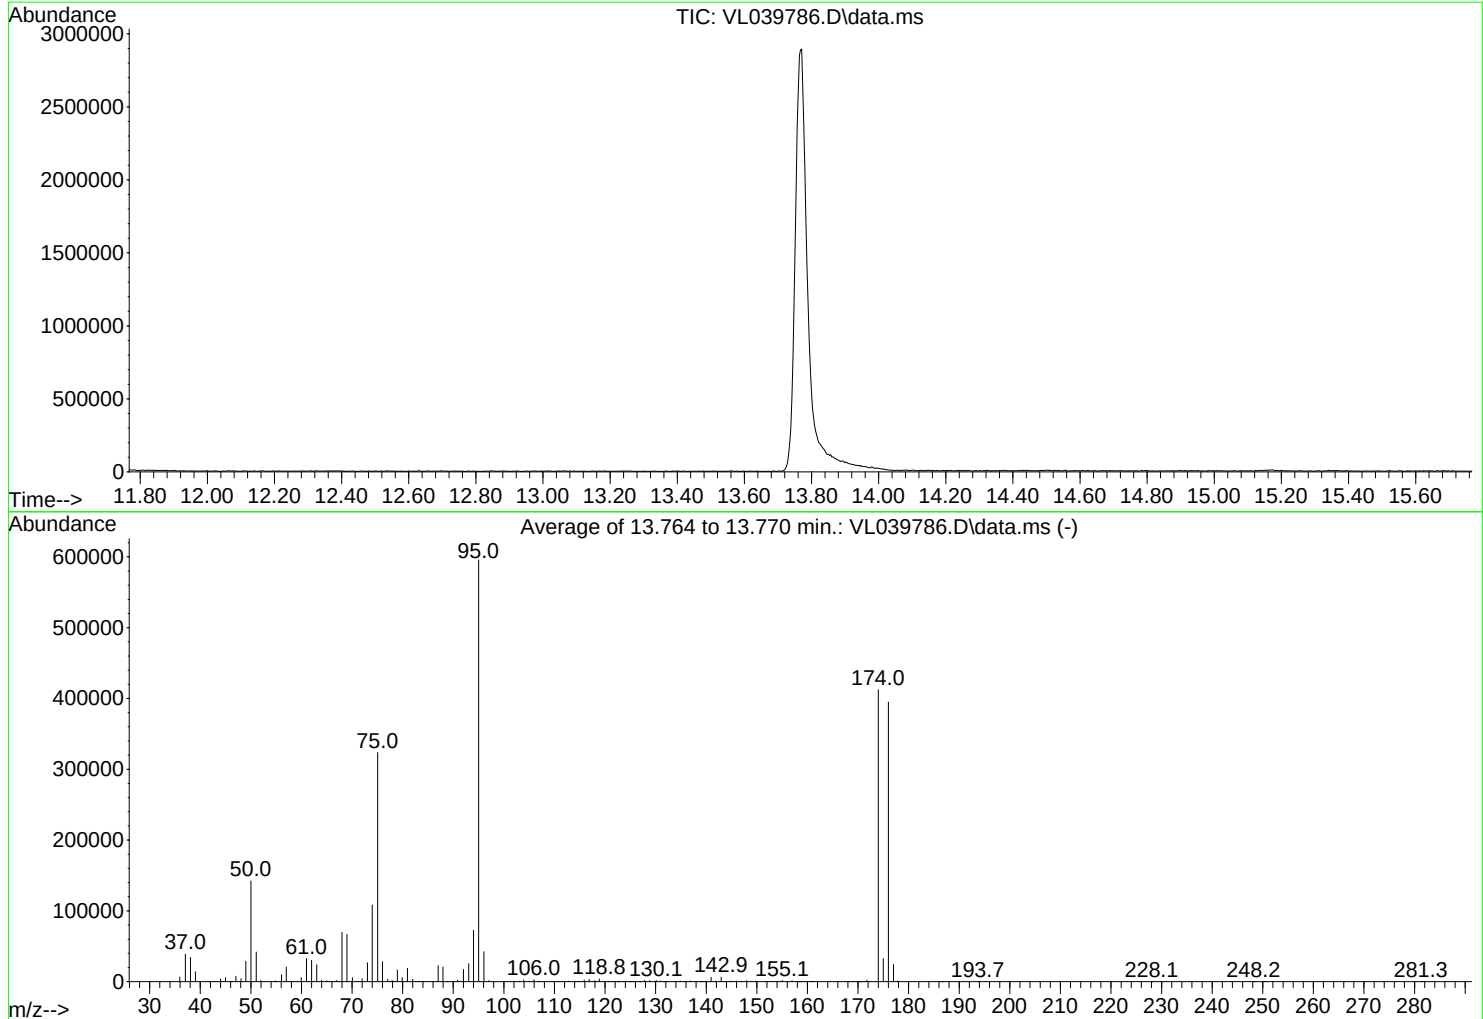

AutoFind: Scans 3471, 3472, 3473; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	142165	PASS
75	95	30	66	54.3	323605	PASS
95	95	100	100	100.0	595776	PASS
96	95	5	9	7.1	42219	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.2	412288	PASS
175	174	4	9	7.9	32387	PASS
176	174	93	101	95.8	394880	PASS
177	176	5	9	6.1	24099	PASS

Average of 13.764 to 13.770 min.: VL039786.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	6292	47.05	7588	58.50	332	66.90	1284
37.05	38915	48.05	4010	59.05	335	67.10	89
38.05	34141	49.00	28694	59.95	5657	68.00	6952
39.05	14024	50.00	142165	61.00	32632	69.00	6680
40.00	284	51.05	41733	62.00	30144	70.05	5645
41.80	138	51.95	1710	63.00	23920	71.05	323
42.80	186	52.30	200	63.95	2099	72.00	4180
43.30	291	54.85	1167	64.95	892	73.05	26768
44.00	3581	56.05	9660	65.20	673	74.00	108176
45.00	5998	57.00	20496	65.90	457	75.05	323605
46.20	334	58.00	927	66.50	287	76.00	28184

Average of 13.764 to 13.770 min.: VL039786.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	3500	87.00	22949	103.05	472	112.85	642
77.90	1857	87.95	20523	103.90	2337	113.90	56
78.10	531	88.80	62	105.00	778	114.55	168
78.95	16438	90.85	2071	105.95	2631	114.90	338
79.90	5590	91.10	406	106.85	441	115.10	332
80.95	18861	92.00	17270	107.20	189	115.90	2151
82.00	3337	93.05	25301	109.55	254	116.85	3095
82.80	246	94.00	72557	110.05	336	117.70	565
83.10	484	95.00	595776	110.80	491	118.05	1429
84.00	287	96.05	42219	111.60	270	118.85	3804
85.80	620	97.05	1316	112.00	443	120.60	82

Average of 13.764 to 13.770 min.: VL039786.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
121.85	167	128.85	1480	138.80	84	145.95	999
122.50	85	129.80	504	139.00	63	146.70	227
122.70	123	130.10	1504	139.90	161	147.00	322
123.70	245	130.95	953	140.10	355	147.95	1677
123.95	498	131.60	56	140.95	6088	148.65	197
124.65	226	132.10	63	141.90	943	149.00	264
125.00	65	133.75	203	142.95	6429	149.80	587
125.60	55	134.85	932	143.75	184	150.00	133
125.95	292	135.95	130	144.00	132	151.80	165
126.90	63	136.85	975	144.60	170	152.10	137
127.85	1838	137.80	163	144.95	596	152.90	387

Average of 13.764 to 13.770 min.: VL039786.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.00	263	161.10	446	171.30	304	248.20	66
154.60	484	162.00	165	171.75	2090	250.30	60
155.05	1557	164.60	134	172.30	573	281.30	59
156.00	171	166.20	155	174.00	412288		
156.95	1174	168.55	312	175.00	32387		
158.40	63	169.20	139	176.00	394880		
158.70	282	169.80	102	177.00	24099		
159.10	284	170.00	52	177.85	1157		
159.90	75	170.40	124	186.70	59		
160.70	389	170.65	273	193.70	88		
160.90	219	171.10	160	228.10	55		