
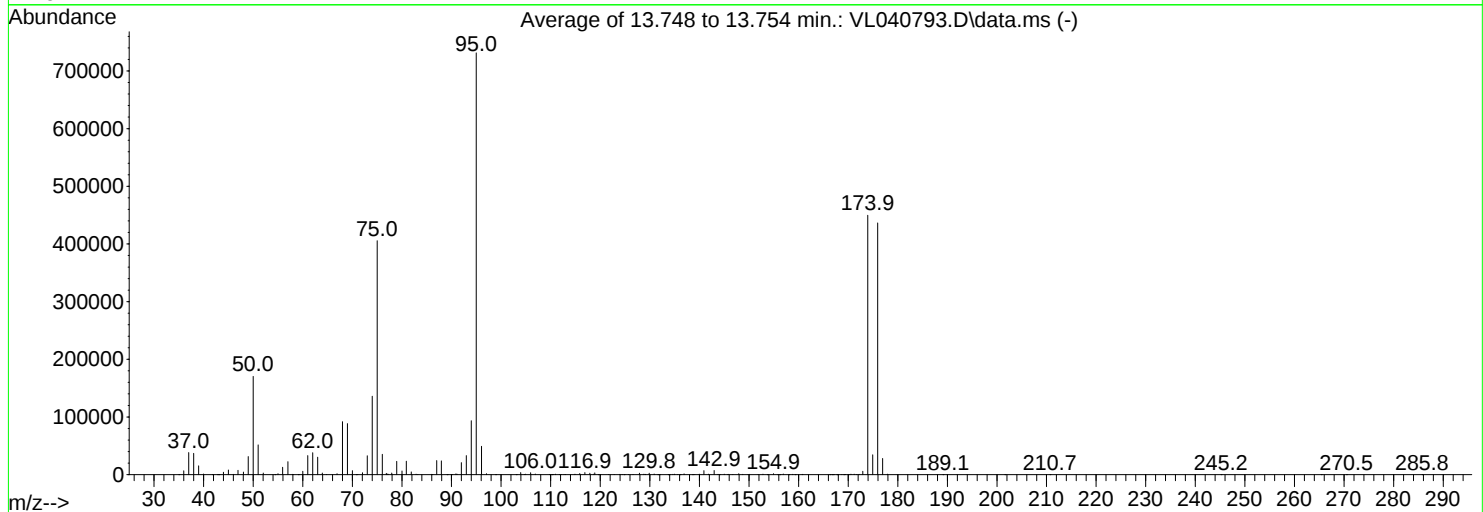


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL102523\
Data File : VL040793.D
Acq On : 25 Oct 2023 9:01
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101123AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Oct 12 00:21:08 2023

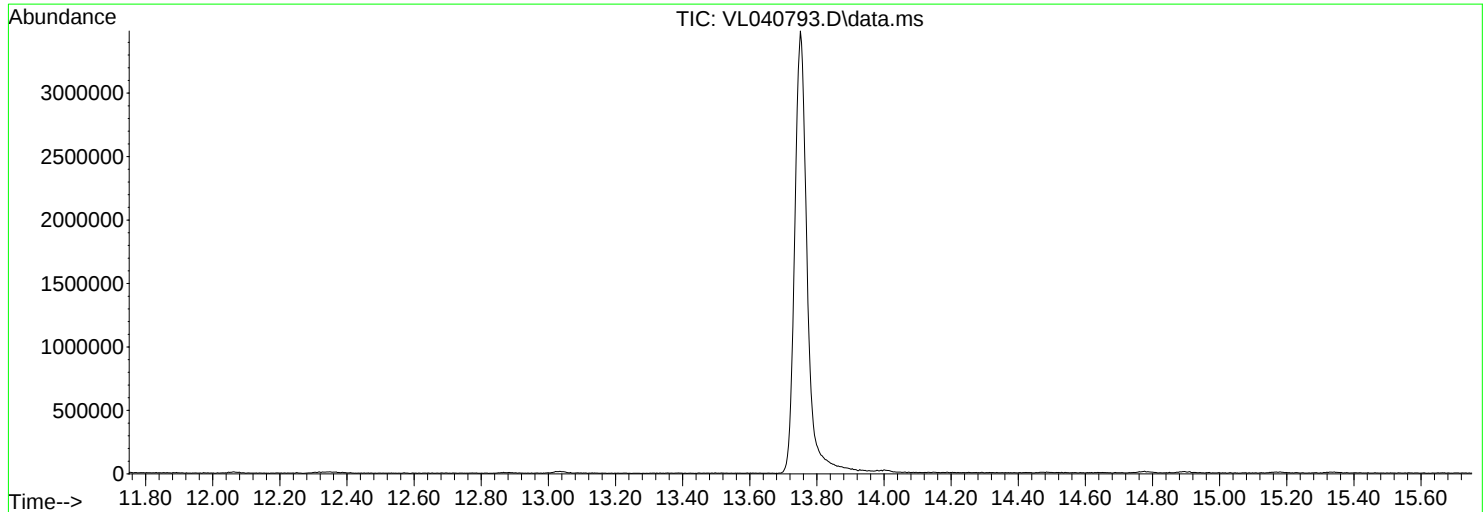

AutoFind: Scans 3466, 3467, 3468; Background Corrected with Scan 3444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.3	170389	PASS
75	95	30	66	55.5	405781	PASS
95	95	100	100	100.0	731456	PASS
96	95	5	9	6.7	49072	PASS
173	174	0.00	2	1.3	5971	PASS
174	95	50	120	61.5	449813	PASS
175	174	4	9	7.7	34432	PASS
176	174	93	101	97.1	436544	PASS
177	176	5	9	6.4	28005	PASS

Average of 13.748 to 13.754 min.: VL040793.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.00	55	46.05	462	57.90	520	69.00	8843
36.00	6731	46.95	7534	58.15	386	70.00	698
37.00	38280	48.05	4524	59.10	57	70.80	12
38.00	36829	49.00	31443	60.00	5912	71.10	17
39.00	15332	50.00	170389	61.00	33093	72.05	3397
40.00	1055	51.00	51624	62.00	37936	73.00	32763
41.80	56	52.05	2697	63.00	30232	74.00	135872
42.80	152	54.40	106	63.95	2669	75.00	405781
43.10	102	55.00	1782	64.80	175	76.05	35325
44.00	4095	55.95	12817	66.90	1541	76.85	2335
45.00	8063	57.00	22589	68.00	91917	77.00	1105

Average of 13.748 to 13.754 min.: VL040793.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.20	844	87.95	23776	98.90	63	110.95	714
77.95	2735	89.10	83	103.05	114	111.75	410
78.95	22957	89.95	113	103.95	3746	112.10	209
80.00	6328	90.90	1379	104.70	391	112.70	175
80.90	23347	91.10	931	104.95	927	113.00	446
81.90	4858	92.00	20901	105.95	3289	114.90	910
82.85	741	93.00	32995	106.90	993	115.85	1852
83.20	204	94.00	93496	109.80	224	116.90	3775
86.00	519	95.00	731456	110.00	172	117.90	2453
86.20	192	96.05	49072	110.20	127	118.70	932
87.00	24323	97.05	1663	110.60	189	118.90	3031

Average of 13.748 to 13.754 min.: VL040793.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.60	84	129.10	514	136.90	1395	145.90	694
120.00	245	129.85	2616	138.60	147	146.75	428
121.70	402	130.85	1039	139.05	188	147.95	1704
122.80	417	131.60	89	139.95	806	148.75	635
123.95	601	131.90	109	140.90	6906	149.80	292
124.40	183	133.70	65	141.85	722	150.05	573
124.80	53	133.90	88	142.95	7323	151.85	165
125.70	234	134.65	691	143.75	535	152.80	735
126.60	162	135.00	753	144.00	122	153.70	146
127.90	2421	135.65	232	145.00	793	153.85	237
128.80	966	136.10	110	145.70	284	154.95	1759

Average of 13.748 to 13.754 min.: VL040793.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.80	54	167.70	65	173.95	449813	285.75	138
156.20	104	167.90	63	174.95	34432		
156.90	1125	168.70	199	175.95	436544		
158.00	72	169.10	114	176.95	28005		
158.80	473	169.45	223	177.90	867		
159.30	50	170.00	141	189.10	125		
160.70	297	170.55	720	201.60	51		
160.85	513	171.20	879	210.70	73		
166.30	62	171.70	348	245.20	50		
166.70	68	172.20	701	265.40	54		
167.00	66	172.95	5971	270.50	57		