

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL102721\
 Data File : VL037912.D
 Acq On : 27 Oct 2021 12:02
 Operator : SY/AP
 Sample : OC102621 CAN 10294
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC102621 CAN 10294

Quant Time: Oct 28 06:16:26 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021
 QLast Update : Mon Oct 04 17:43:54 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.69	49	1462023	10.00	ppbv	0.02
33) 1,4-Difluorobenzene	7.19	114	4370874	10.00	ppbv	0.02
55) Chlorobenzene-d5	12.11	117	3606787	10.00	ppbv	0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.44	95	2413863	9.57	ppbv	0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	95.70%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL102721\
Data File : VL037912.D
Acq On : 27 Oct 2021 12:02
Operator : SY/AP
Sample : OC102621 CAN 10294
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC102621 CAN 10294

Quant Time: Oct 28 06:16:26 2021
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021
QLast Update : Mon Oct 04 17:43:54 2021
Response via : Initial Calibration

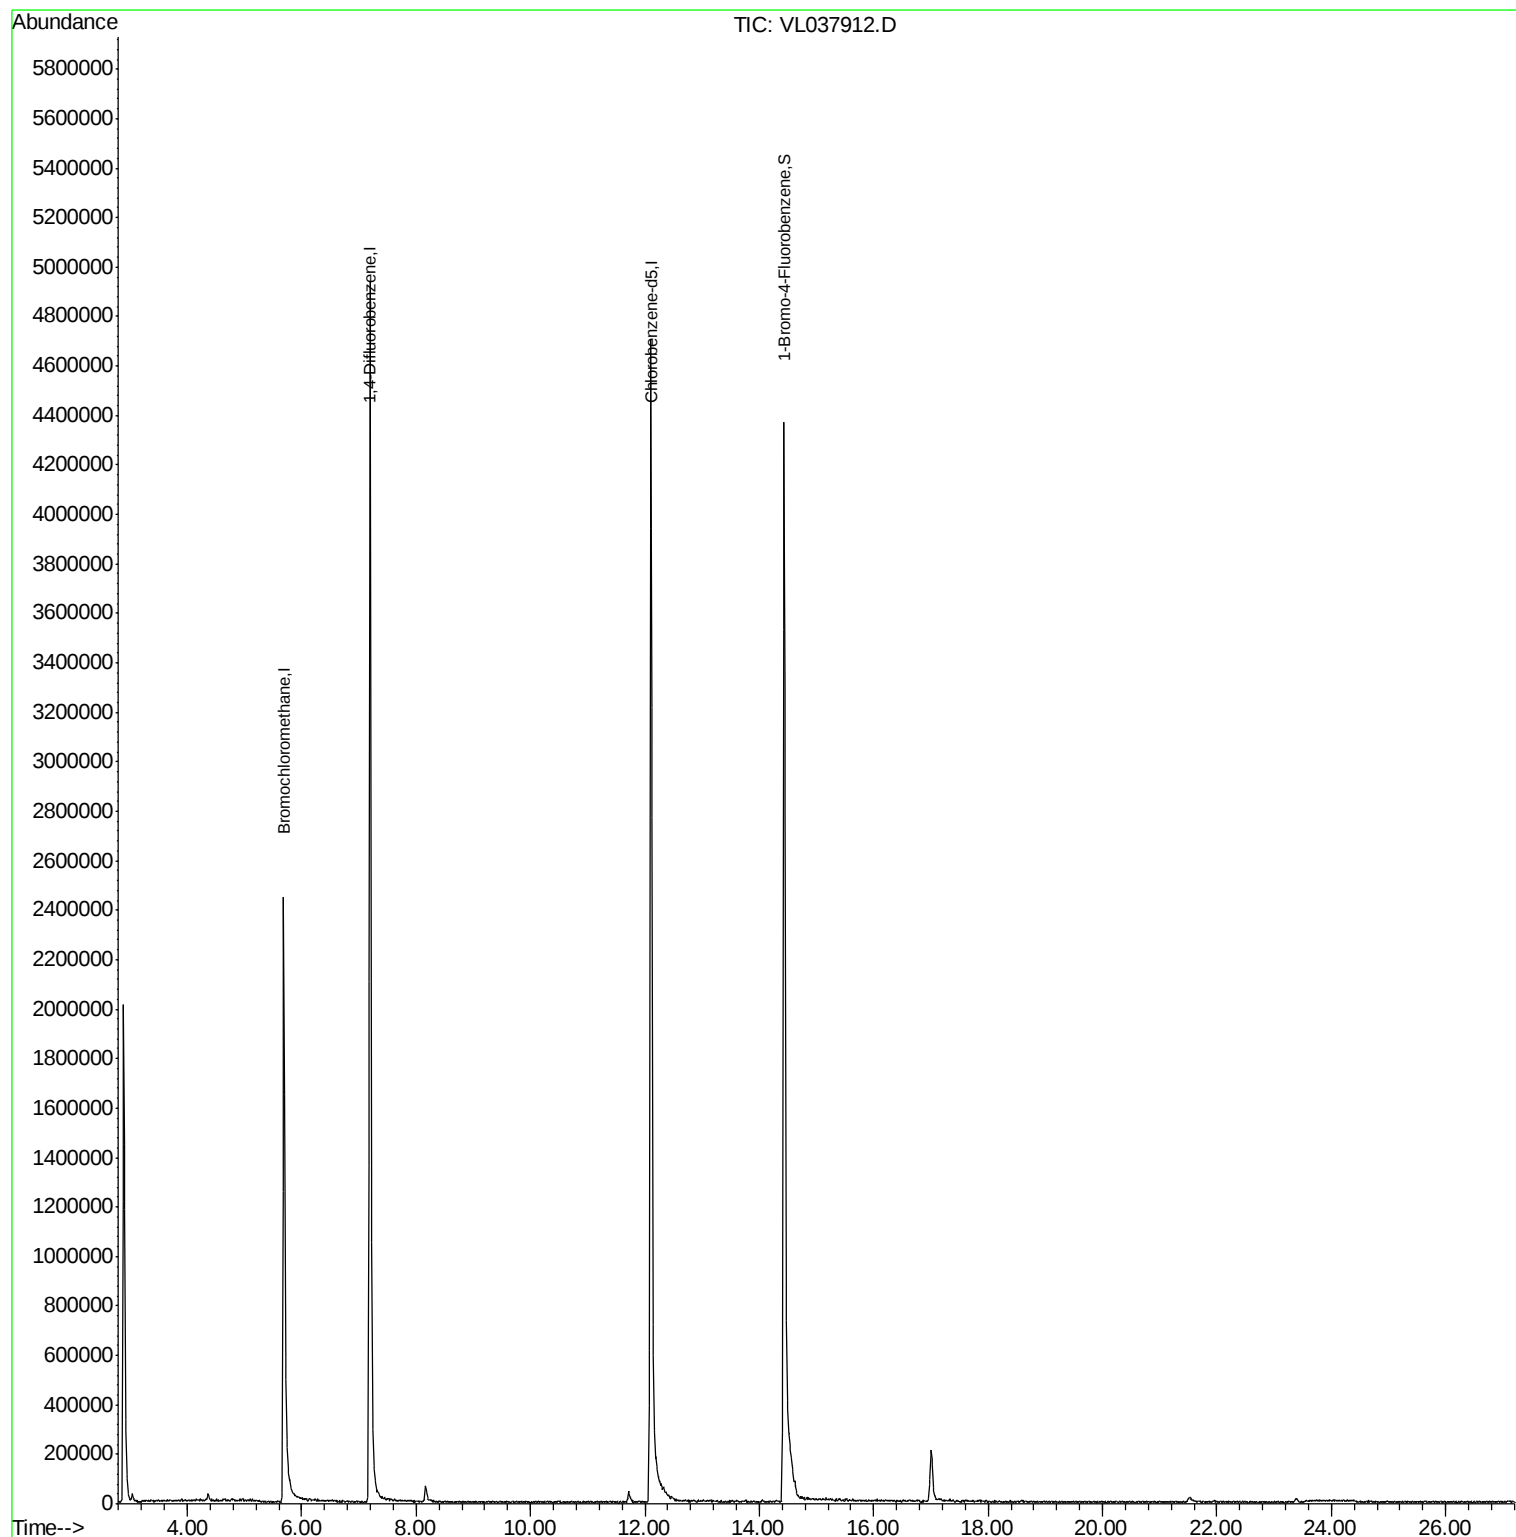

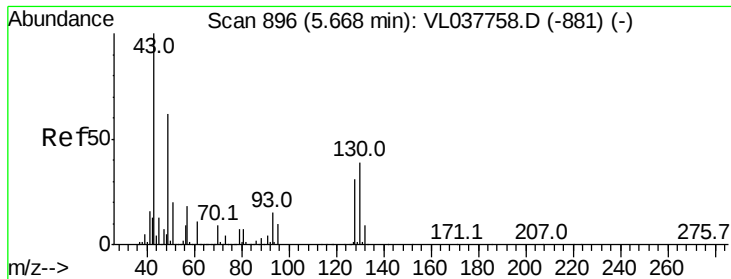

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.69 Instrument: MSVOA_1

Delta R.T. 0.02 min

Lab File: ClientSampleId: QC102621 CAN 10294

Acq: 27 Oct 2021 12:02


Tot Ion: 49 Resp: 1462023

Ion Ratio Lower Upper

49 100

128 55.2 27.1 81.3




130 71.8 33.2 99.6

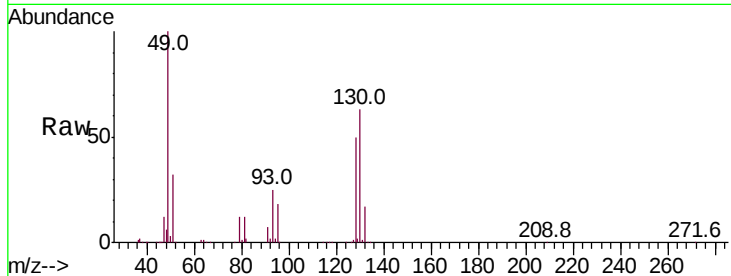

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

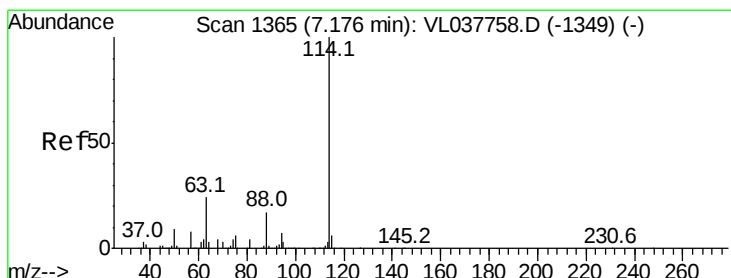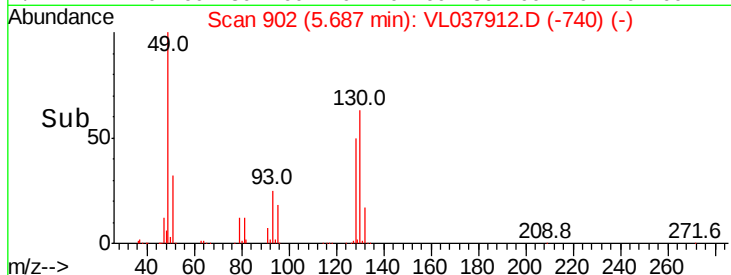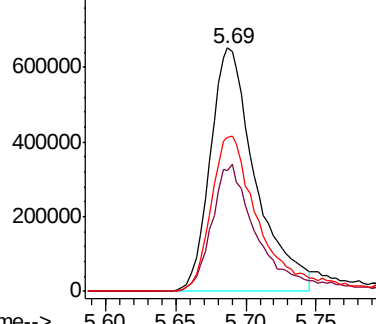

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.19 min Scan# 1371

Delta R.T. 0.02 min

Lab File: VL037912.D

Acq: 27 Oct 2021 12:02


Tgt Ion: 114 Resp: 4370874

Ion Ratio Lower Upper

114 100

63 23.9 19.4 29.2



88 18.0 14.4 21.6

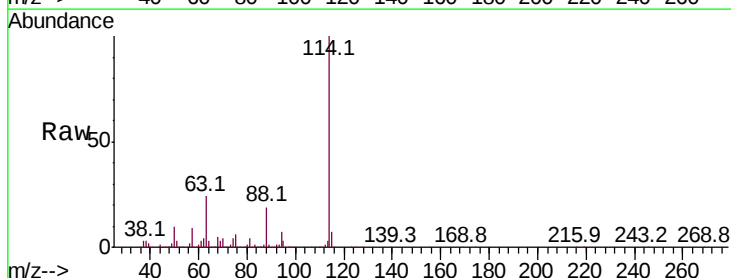


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



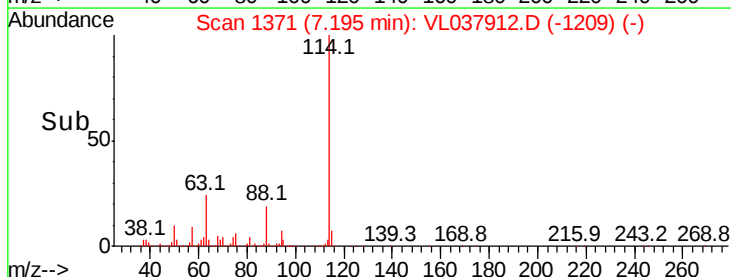
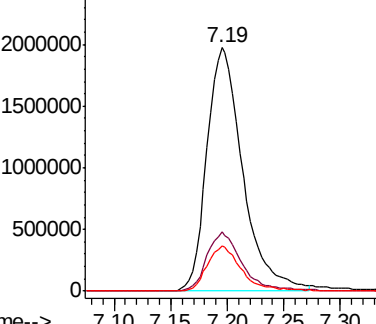


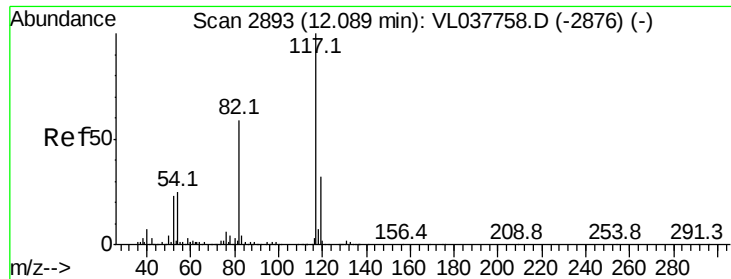

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.11 min
Instrument: MSVOA_1
Delta R.T.: 0.02 min
Lab File: ClientSampleId : QC102621 CAN 10294
Acq: 27 Oct 2021 12:02

Tot Ion: 117 Resp: 3606787

Ion	Ratio	Lower	Upper
117	100		
82	65.2	52.2	78.2
119	35.5	26.0	39.0

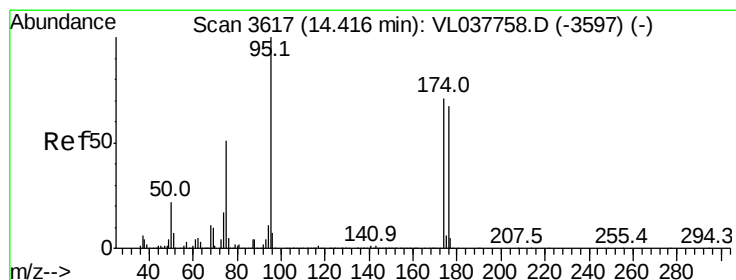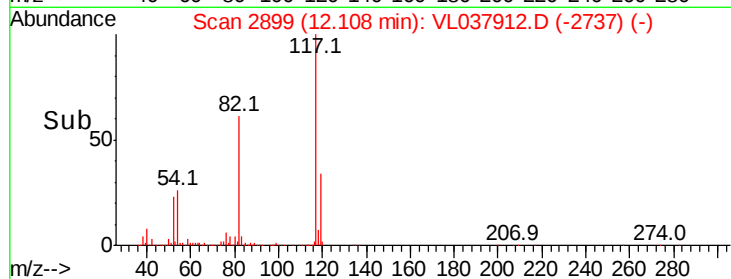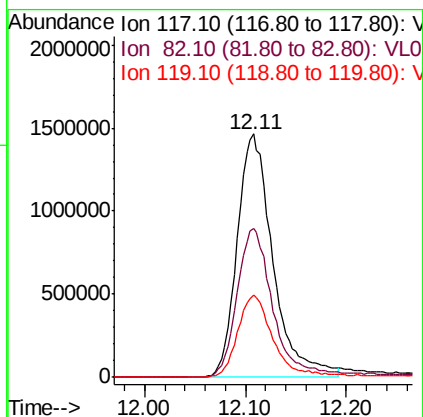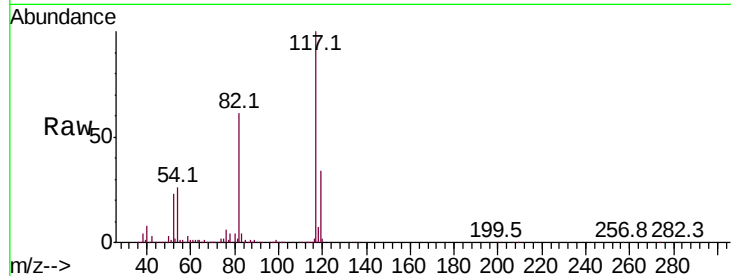

#68
1-Bromo-4-Fluorobenzene
Concen: 9.570 ppbv
RT: 14.44 min Scan# 3623
Delta R.T.: 0.02 min
Lab File: VL037912.D
Acq: 27 Oct 2021 12:02

Tgt Ion: 95 Resp: 2413863

Ion	Ratio	Lower	Upper
95	100		
174	78.3	57.8	86.6
175	5.7	4.7	7.1

