


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL102721\
 Data File : VL037908.D
 Acq On : 27 Oct 2021 8:31
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021
 Last Update : Mon Oct 04 17:43:54 2021

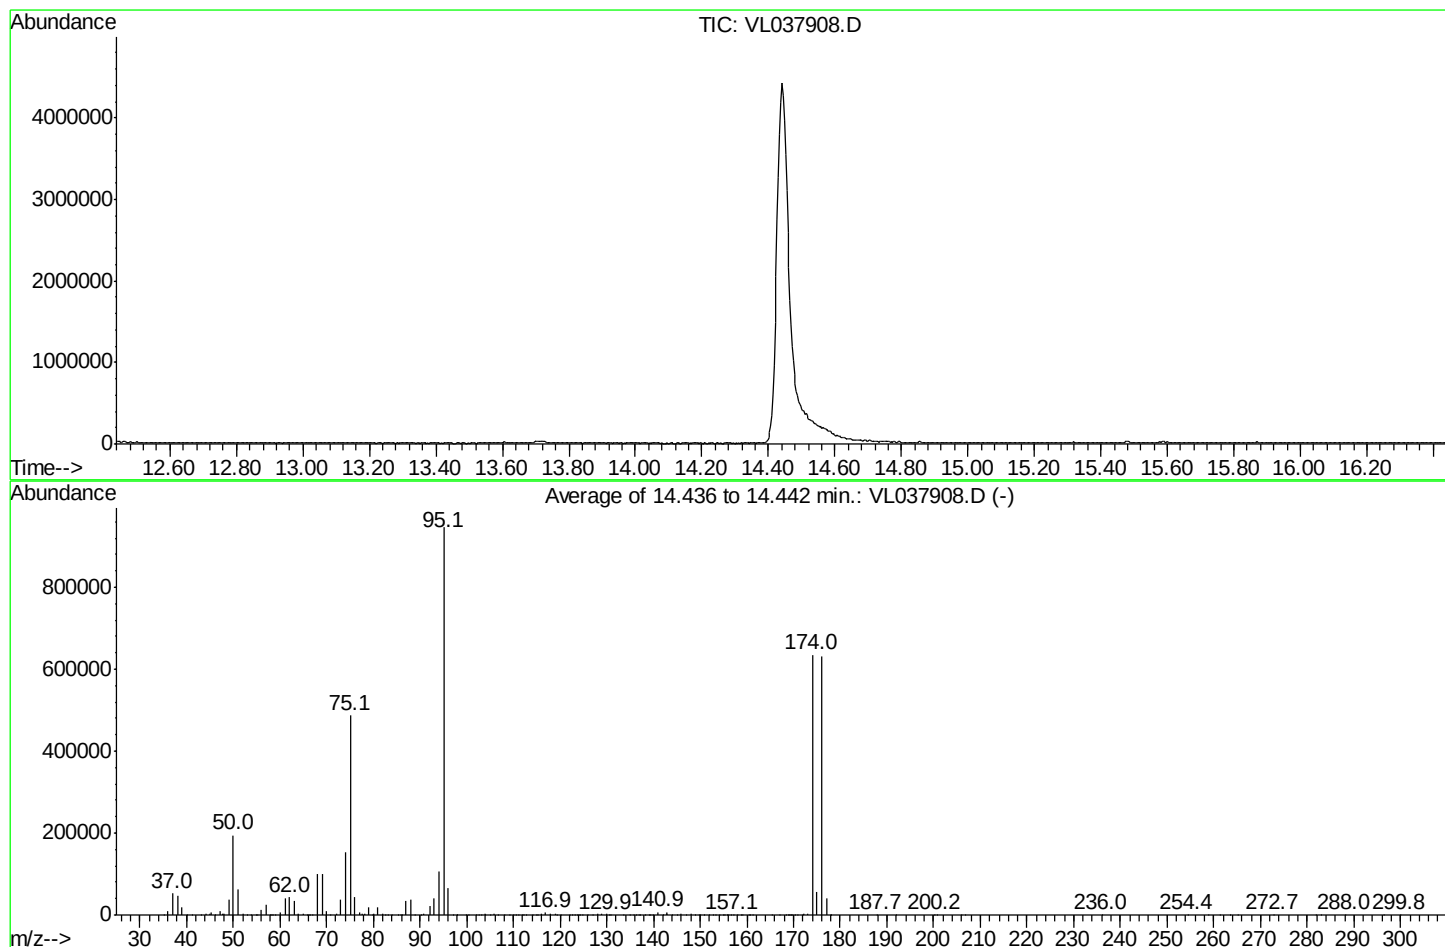

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.6	195157	PASS
75	95	30	66	51.4	486144	PASS
95	95	100	100	100.0	946368	PASS
96	95	5	9	6.8	64296	PASS
173	174	0.00	2	0.5	3412	PASS
174	95	50	120	67.2	635776	PASS
175	174	4	9	8.8	55669	PASS
176	174	93	101	99.5	632554	PASS
177	176	5	9	6.5	40970	PASS