


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL103018\
 Data File : VL032698.D
 Acq On : 30 Oct 2018 12:49
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL101818AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Oct 25 05:15:43 2018
 Last Update : Thu Oct 25 05:15:43 2018

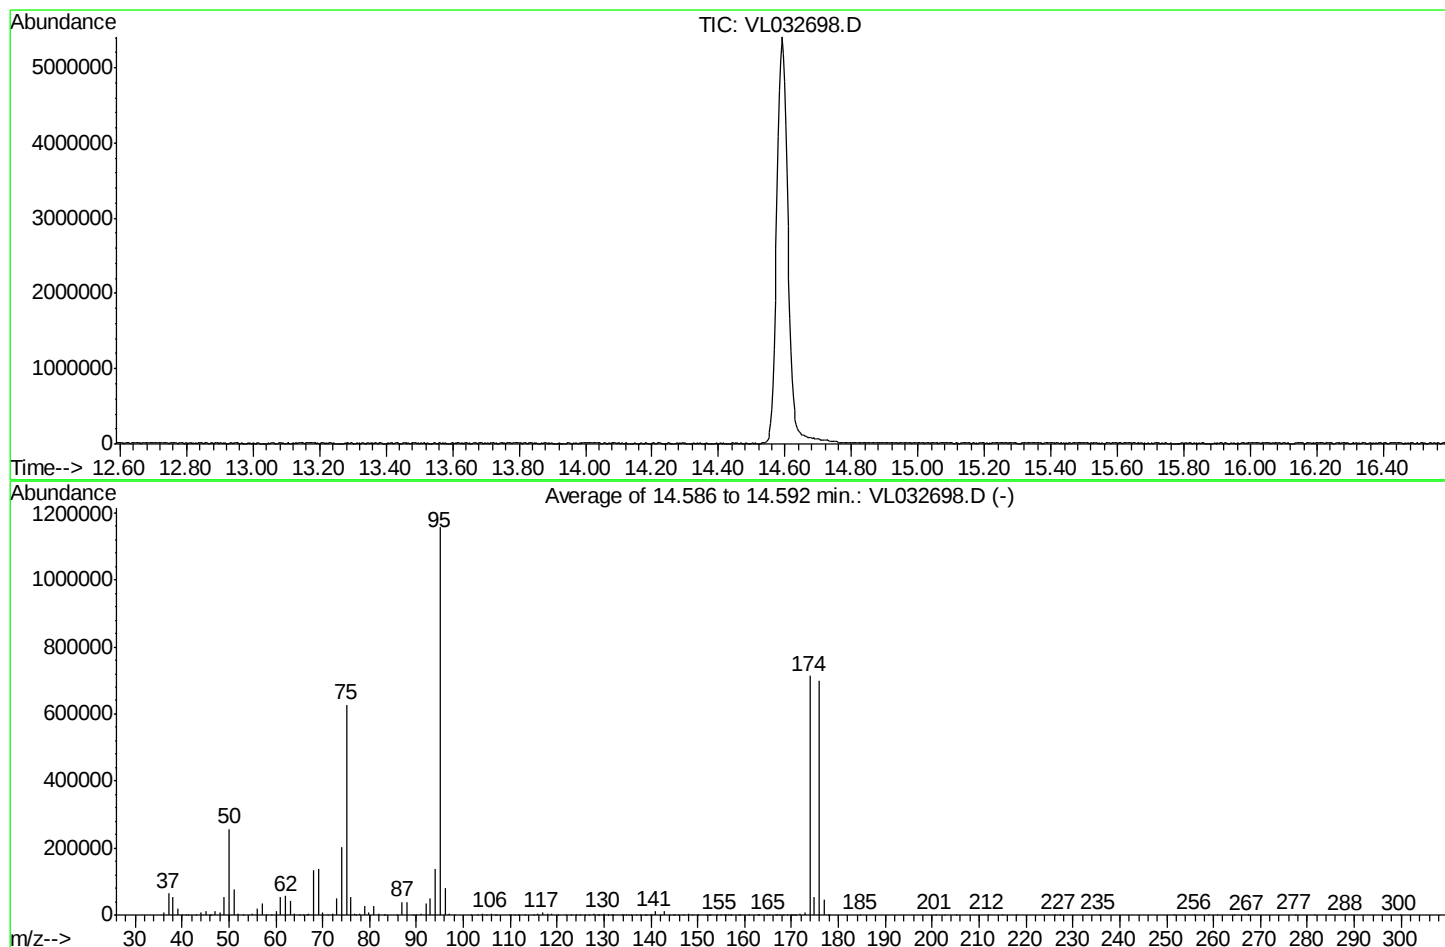

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.3	257450	PASS
75	95	30	66	54.2	627498	PASS
95	95	100	100	100.0	1156948	PASS
96	95	5	9	7.0	80624	PASS
173	174	0.00	2	1.1	7946	PASS
174	95	50	120	61.7	713792	PASS
175	174	4	9	7.5	53250	PASS
176	174	93	101	98.2	700714	PASS
177	176	5	9	6.4	44832	PASS