


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110121\
 Data File : VL037932.D
 Acq On : 1 Nov 2021 8:07
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL110121AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Nov 02 05:54:07 2021
 Last Update : Tue Nov 02 05:54:07 2021

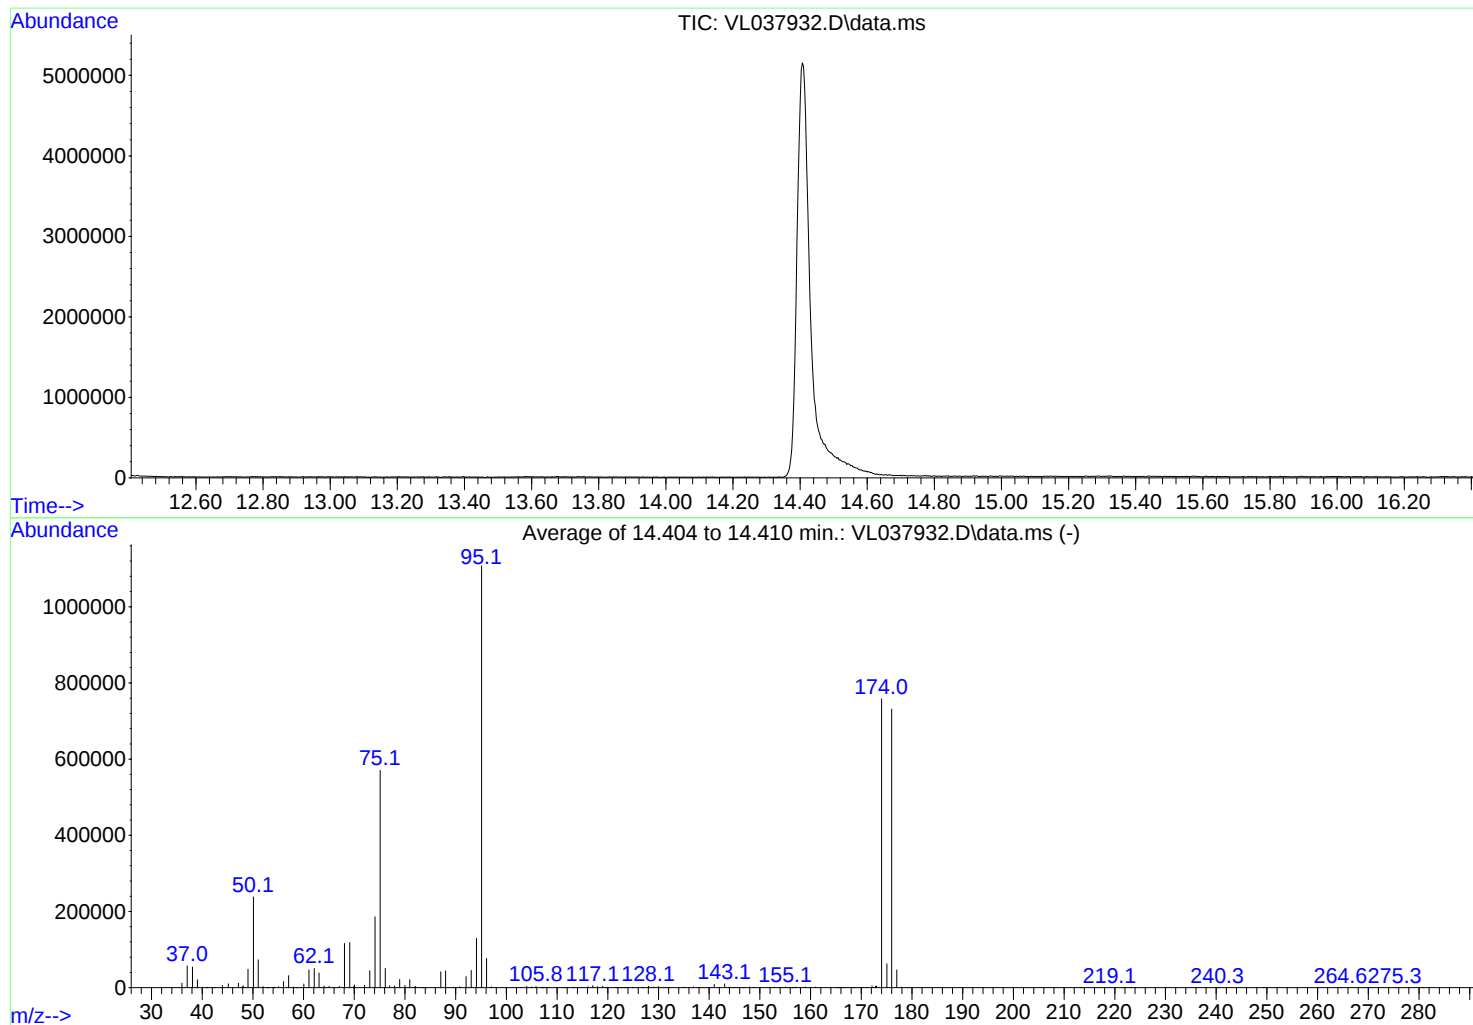

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.5	238293	PASS
75	95	30	66	51.5	570645	PASS
95	95	100	100	100.0	1107456	PASS
96	95	5	9	6.9	76672	PASS
173	174	0.00	2	0.5	4042	PASS
174	95	50	120	68.5	758507	PASS
175	174	4	9	8.3	62597	PASS
176	174	93	101	96.4	731526	PASS
177	176	5	9	6.4	46725	PASS

Average of 14.404 to 14.410 min.: VL037932.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	11944	47.90	1965	57.05	31477	68.05	11588
37.05	57256	48.10	4952	58.00	1775	69.10	11869
38.10	54336	49.05	48160	58.60	84	69.90	281
39.05	20477	50.10	238293	60.05	9850	70.05	701
40.10	1128	51.05	73296	61.05	46875	71.10	319
40.85	118	52.00	2796	62.10	50533	72.00	5776
42.30	73	52.90	248	63.05	38747	73.05	44427
44.00	5502	53.15	633	64.05	4221	74.10	186027
45.15	10118	54.15	182	65.05	3436	75.10	570645
46.05	939	55.05	2576	65.95	671	76.10	50544
47.15	11990	56.05	16028	67.05	3557	76.95	5289

Average of 14.404 to 14.410 min.: VL037932.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.90	4328	88.00	44093	104.00	3502	111.50	54
78.95	21440	89.50	137	105.05	1700	111.90	100
80.00	6082	90.80	2454	105.85	3567	112.15	631
80.95	20896	91.00	846	106.85	784	112.75	625
81.85	1274	92.05	29205	107.00	186	113.20	142
82.10	3219	93.05	45560	107.20	157	114.00	53
83.05	563	94.10	129307	107.75	165	114.85	404
83.50	225	95.10	1.10746e+006	108.50	354	116.00	2221
84.05	235	96.10	76672	110.10	286	116.20	1104
85.95	654	97.05	1942	111.00	447	117.05	5373
87.05	41496	102.80	441	111.20	492	117.95	2720

Average of 14.404 to 14.410 min.: VL037932.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.00	4016	126.80	146	135.80	368	145.00	980
119.70	56	128.05	3857	136.90	1920	145.60	922
121.60	70	129.05	1874	138.00	103	146.05	800
121.90	282	129.95	2858	138.70	456	146.70	57
122.60	175	131.00	750	139.65	442	147.05	605
122.85	311	131.20	541	140.20	642	147.95	2310
123.20	84	131.60	83	141.00	8890	148.70	570
123.60	121	131.90	171	141.95	1121	148.95	765
124.00	823	133.90	167	143.05	9828	149.80	321
124.80	120	134.70	284	143.85	667	150.10	585
126.00	503	135.05	1531	144.65	367	152.00	837

Average of 14.404 to 14.410 min.: VL037932.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
152.90	1463	158.95	1724	168.60	122	176.00	731526
153.75	669	159.85	223	169.00	800	177.00	46725
154.10	141	160.95	1641	169.60	291	177.95	1179
154.70	645	163.90	364	169.90	352	179.05	146
155.10	2278	165.20	58	170.30	767	213.20	62
155.70	71	165.60	62	171.10	770	219.05	336
156.05	278	165.90	163	172.10	4555	221.50	140
156.40	140	166.40	162	172.80	3221	222.00	63
157.05	1771	166.80	263	173.00	4042	223.10	95
157.90	104	167.35	342	174.00	758507	230.00	55
158.10	412	168.30	191	175.05	62597	240.30	121

Average of 14.404 to 14.410 min.: VL037932.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
249.30	68						
264.60	53						
269.00	201						
270.10	127						
275.30	217						
280.80	66						