


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110221\
 Data File : VL037962.D
 Acq On : 2 Nov 2021 8:55
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL110121AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Nov 02 05:54:07 2021
 Last Update : Tue Nov 02 05:54:07 2021

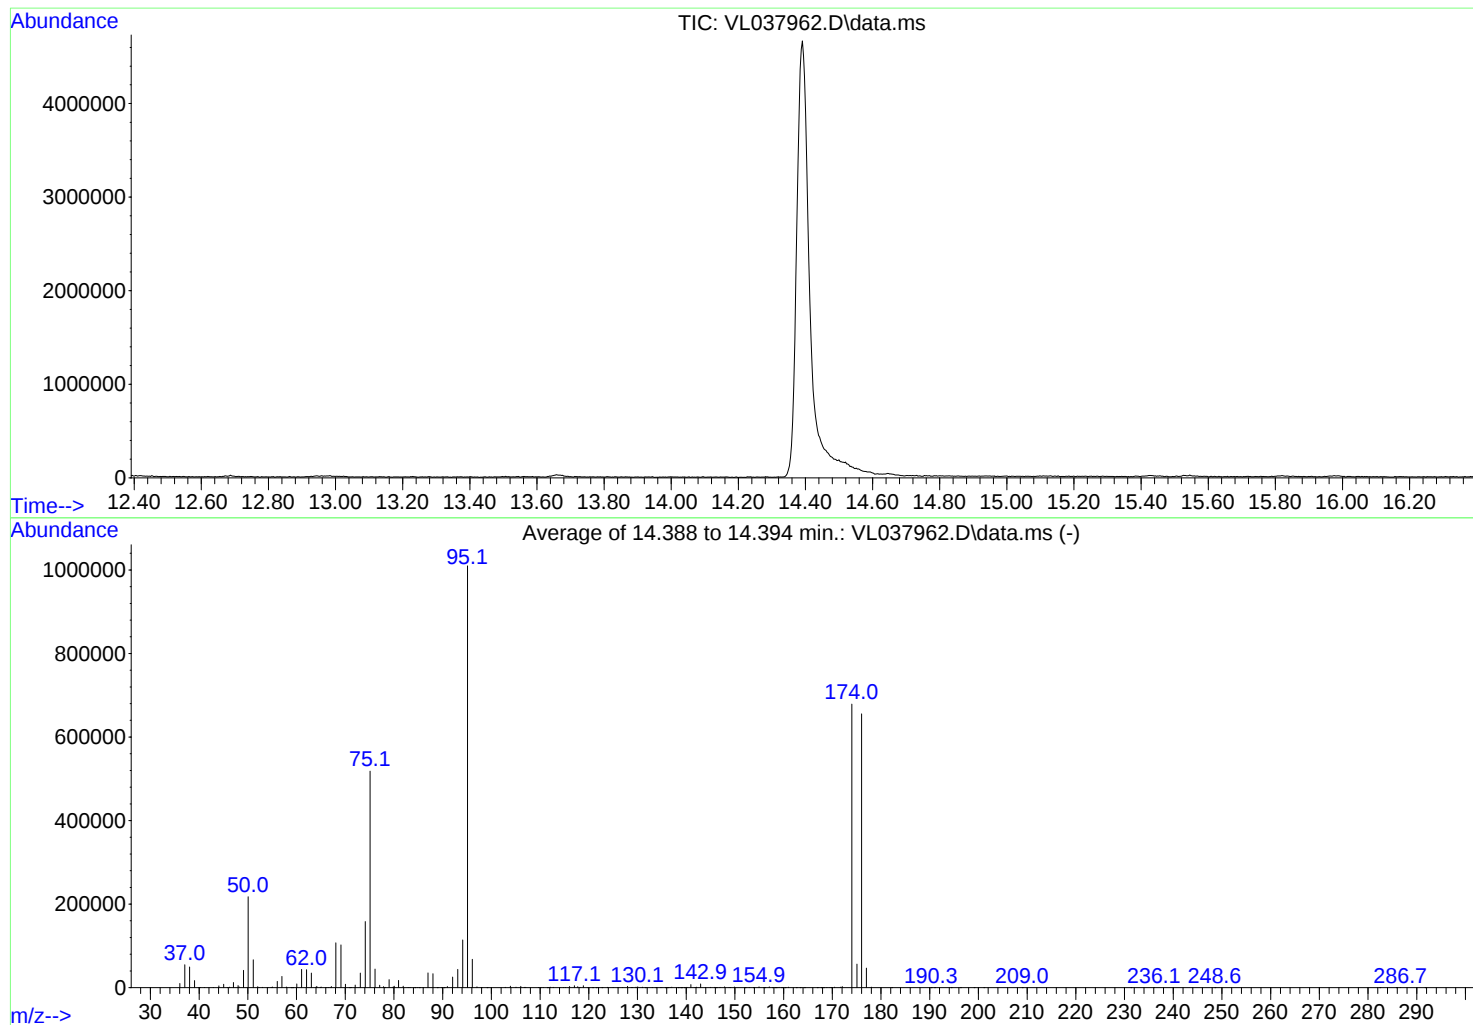

AutoFind: Scans 3608, 3609, 3610; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.6	217664	PASS
75	95	30	66	51.3	518549	PASS
95	95	100	100	100.0	1009941	PASS
96	95	5	9	6.7	67757	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.2	678891	PASS
175	174	4	9	8.3	56451	PASS
176	174	93	101	96.6	655595	PASS
177	176	5	9	7.2	46885	PASS

Average of 14.388 to 14.394 min.: VL037962.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	10148	46.25	1113	54.80	792	64.00	1341
37.05	54787	47.05	12331	55.05	1599	64.15	3231
38.05	49379	48.00	5168	56.05	15131	64.90	311
39.05	16930	48.20	2031	57.00	26768	65.05	148
39.90	35	49.10	41597	57.90	1478	66.05	312
40.20	374	50.05	217664	58.90	107	66.50	334
41.10	346	51.10	66624	59.20	85	66.90	442
42.90	432	52.05	2331	60.05	8650	67.15	2600
44.05	4101	52.30	582	61.05	43691	68.05	107312
45.05	8213	53.00	688	62.05	43131	69.10	102421
45.80	329	54.15	313	63.05	34888	70.05	7916

Average of 14.388 to 14.394 min.: VL037962.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
70.90	104	79.00	19099	86.00	290	96.10	67757
71.30	454	79.80	1121	87.00	35376	97.05	1951
72.05	6310	79.90	1753	88.00	33392	97.90	86
73.10	34845	80.05	3372	88.90	107	99.10	74
74.10	158080	80.95	17117	89.80	126	102.85	897
75.10	518549	81.90	3452	90.30	171	103.90	3556
76.10	44541	82.90	522	90.95	2744	105.05	1125
77.05	5641	83.30	347	92.05	25424	106.05	3280
77.85	2258	84.30	90	93.10	43555	106.75	828
78.00	900	84.90	488	94.10	114197	107.05	872
78.20	908	85.20	128	95.10	1.00994e+006	109.70	284

Average of 14.388 to 14.394 min.: VL037962.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
110.00	69	117.75	2254	126.95	336	135.00	424
110.65	477	118.20	929	127.95	3241	135.70	222
111.50	69	118.90	4496	128.80	301	135.90	140
111.80	311	119.80	114	129.00	319	136.20	70
112.10	1161	120.80	210	129.70	1032	136.70	296
112.70	986	121.50	100	130.05	1797	137.05	1024
114.05	290	121.95	317	131.00	1065	138.35	252
114.85	567	122.70	55	131.60	90	138.90	253
115.20	318	123.85	831	133.05	269	139.10	252
116.05	2717	125.00	286	133.75	217	139.60	235
117.05	4712	126.00	409	134.80	413	140.15	721

Average of 14.388 to 14.394 min.: VL037962.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
140.95	7384	148.80	343	157.70	144	167.70	103
141.80	360	149.10	305	158.20	193	167.95	380
142.10	1096	149.90	1534	158.50	240	168.20	51
142.95	8675	152.10	217	159.05	898	168.90	303
143.95	293	152.95	625	159.60	128	169.55	571
145.00	995	153.80	201	160.30	147	169.80	216
145.85	933	154.00	329	161.00	1209	170.45	1237
146.00	453	154.95	2051	162.60	222	171.70	1145
146.20	98	155.90	246	163.40	83	172.05	2722
146.95	982	156.10	209	164.30	52	174.00	678891
147.90	2005	157.05	2014	166.90	113	175.05	56451

Average of 14.388 to 14.394 min.: VL037962.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.00	655595	231.30	94				
177.00	46885	236.10	302				
178.00	1121	248.55	196				
182.20	50	282.40	67				
190.30	73	285.80	105				
191.00	54	286.70	278				
194.40	51	291.70	117				

196.30	69
199.10	57
201.10	60
209.00	72

Instrument :
MSVOA_L
ClientSampleId :
BFB