

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL110320\
 Data File : VL035820.D
 Acq On : 4 Nov 2020 1:51
 Operator : SY/AP
 Sample : L4610-01 10X
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV1

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 3
 Start Thrs: 0.001
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.851	6	20	56	rBV	2290454	5089864	7.69%	1.106%
2	5.639	871	887	933	rBV	2844229	6675486	10.08%	1.450%
3	7.144	1337	1355	1399	rBV	5096907	11405718	17.22%	2.478%
4	12.060	2859	2884	2910	rBV	5738337	13890574	20.97%	3.018%
5	13.548	3313	3347	3367	rBV6	299045	1012461	1.53%	0.220%
6	14.391	3586	3609	3648	rBV	6137003	15085787	22.78%	3.278%
7	15.153	3820	3846	3860	rBV6	468655	1700617	2.57%	0.369%
8	15.417	3907	3928	3938	rBV6	321385	1087369	1.64%	0.236%
9	15.484	3938	3949	3961	rVV3	510818	1226566	1.85%	0.266%
10	15.728	4007	4025	4044	rBV7	400753	1262190	1.91%	0.274%
11	15.835	4044	4058	4079	rVB5	291154	914200	1.38%	0.199%
12	16.108	4118	4143	4165	rVB	8974602	24632836	37.20%	5.352%
13	16.285	4192	4198	4217	rVB5	243053	689926	1.04%	0.150%
14	16.420	4217	4240	4250	rBV2	1096142	3024528	4.57%	0.657%
15	16.500	4250	4265	4280	rVV2	4050799	10928455	16.50%	2.374%
16	16.574	4280	4288	4295	rVV2	753599	1738167	2.62%	0.378%
17	16.638	4295	4308	4317	rVV3	2534601	7079803	10.69%	1.538%
18	16.687	4317	4323	4344	rVB	1641024	3872889	5.85%	0.841%
19	16.809	4349	4361	4387	rVB8	343322	1144507	1.73%	0.249%
20	16.963	4387	4409	4419	rBV2	1169404	3465880	5.23%	0.753%
21	17.040	4419	4433	4448	rVV4	3278528	10340031	15.61%	2.247%
22	17.117	4448	4457	4480	rVB2	2143820	5805499	8.77%	1.261%
23	17.253	4480	4499	4527	rVB5	2017188	6116297	9.24%	1.329%
24	17.674	4608	4630	4645	rBV3	2876875	8893800	13.43%	1.932%
25	17.754	4645	4655	4673	rVB5	398231	1217757	1.84%	0.265%
26	17.924	4688	4708	4730	rBV	12816169	38570263	58.24%	8.380%
27	18.015	4730	4736	4759	rVB2	616966	1449710	2.19%	0.315%
28	18.166	4759	4783	4801	rBV	6896708	20497330	30.95%	4.453%
29	18.349	4818	4840	4879	rBV2	18073228	66225424	100.00%	14.389%
30	18.539	4879	4899	4928	rVB3	1182295	4204453	6.35%	0.914%
31	18.699	4928	4949	4963	rBV3	2541501	6924126	10.46%	1.504%
32	18.802	4963	4981	4995	rVV5	4316497	14163078	21.39%	3.077%
33	18.896	4995	5010	5041	rVV2	13315720	51196708	77.31%	11.124%
34	19.053	5041	5059	5087	rVV	10895161	32751950	49.46%	7.116%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL110320\
Data File : VL035820.D
Acq On : 4 Nov 2020 1:51
Operator : SY/AP
Sample : L4610-01 10X
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV1

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 3 Min Area: 3 % of largest Peak
Start Thrs: 0.001 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Nov 04 02:40:06 2020

35	19.198	5087	5104	5119	rVV6	2428069	7149740	10.80%	1.553%
36	19.314	5131	5140	5151	rVV4	526208	1272783	1.92%	0.277%
37	19.449	5151	5182	5211	rVB3	8738177	31433265	47.46%	6.830%
38	19.629	5211	5238	5250	rBV3	1033190	4356537	6.58%	0.947%
39	19.722	5250	5267	5282	rVV5	1733302	6535144	9.87%	1.420%
40	19.805	5282	5293	5308	rVV2	2053227	5206049	7.86%	1.131%
41	19.973	5326	5345	5356	rBV6	1594830	5802027	8.76%	1.261%
42	20.018	5358	5359	5387	rVB4	1175827	2551851	3.85%	0.554%
43	20.172	5387	5407	5430	rVB7	435930	1777913	2.68%	0.386%
44	20.400	5462	5478	5510	rVB4	1162882	4035641	6.09%	0.877%
45	20.561	5510	5528	5537	rVV3	334851	875248	1.32%	0.190%
46	20.625	5537	5548	5553	rVV9	321649	826630	1.25%	0.180%
47	20.677	5553	5564	5602	rVB4	688998	2613477	3.95%	0.568%
48	20.982	5645	5659	5680	rVB5	247866	801665	1.21%	0.174%
49	21.979	5951	5969	5985	rBV3	212488	730695	1.10%	0.159%


Sum of corrected areas: 460252914

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL110320\
Data File : VL035820.D
Acq On : 4 Nov 2020 1:51
Operator : SY/AP
Sample : L4610-01 10X
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampled :
SV1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

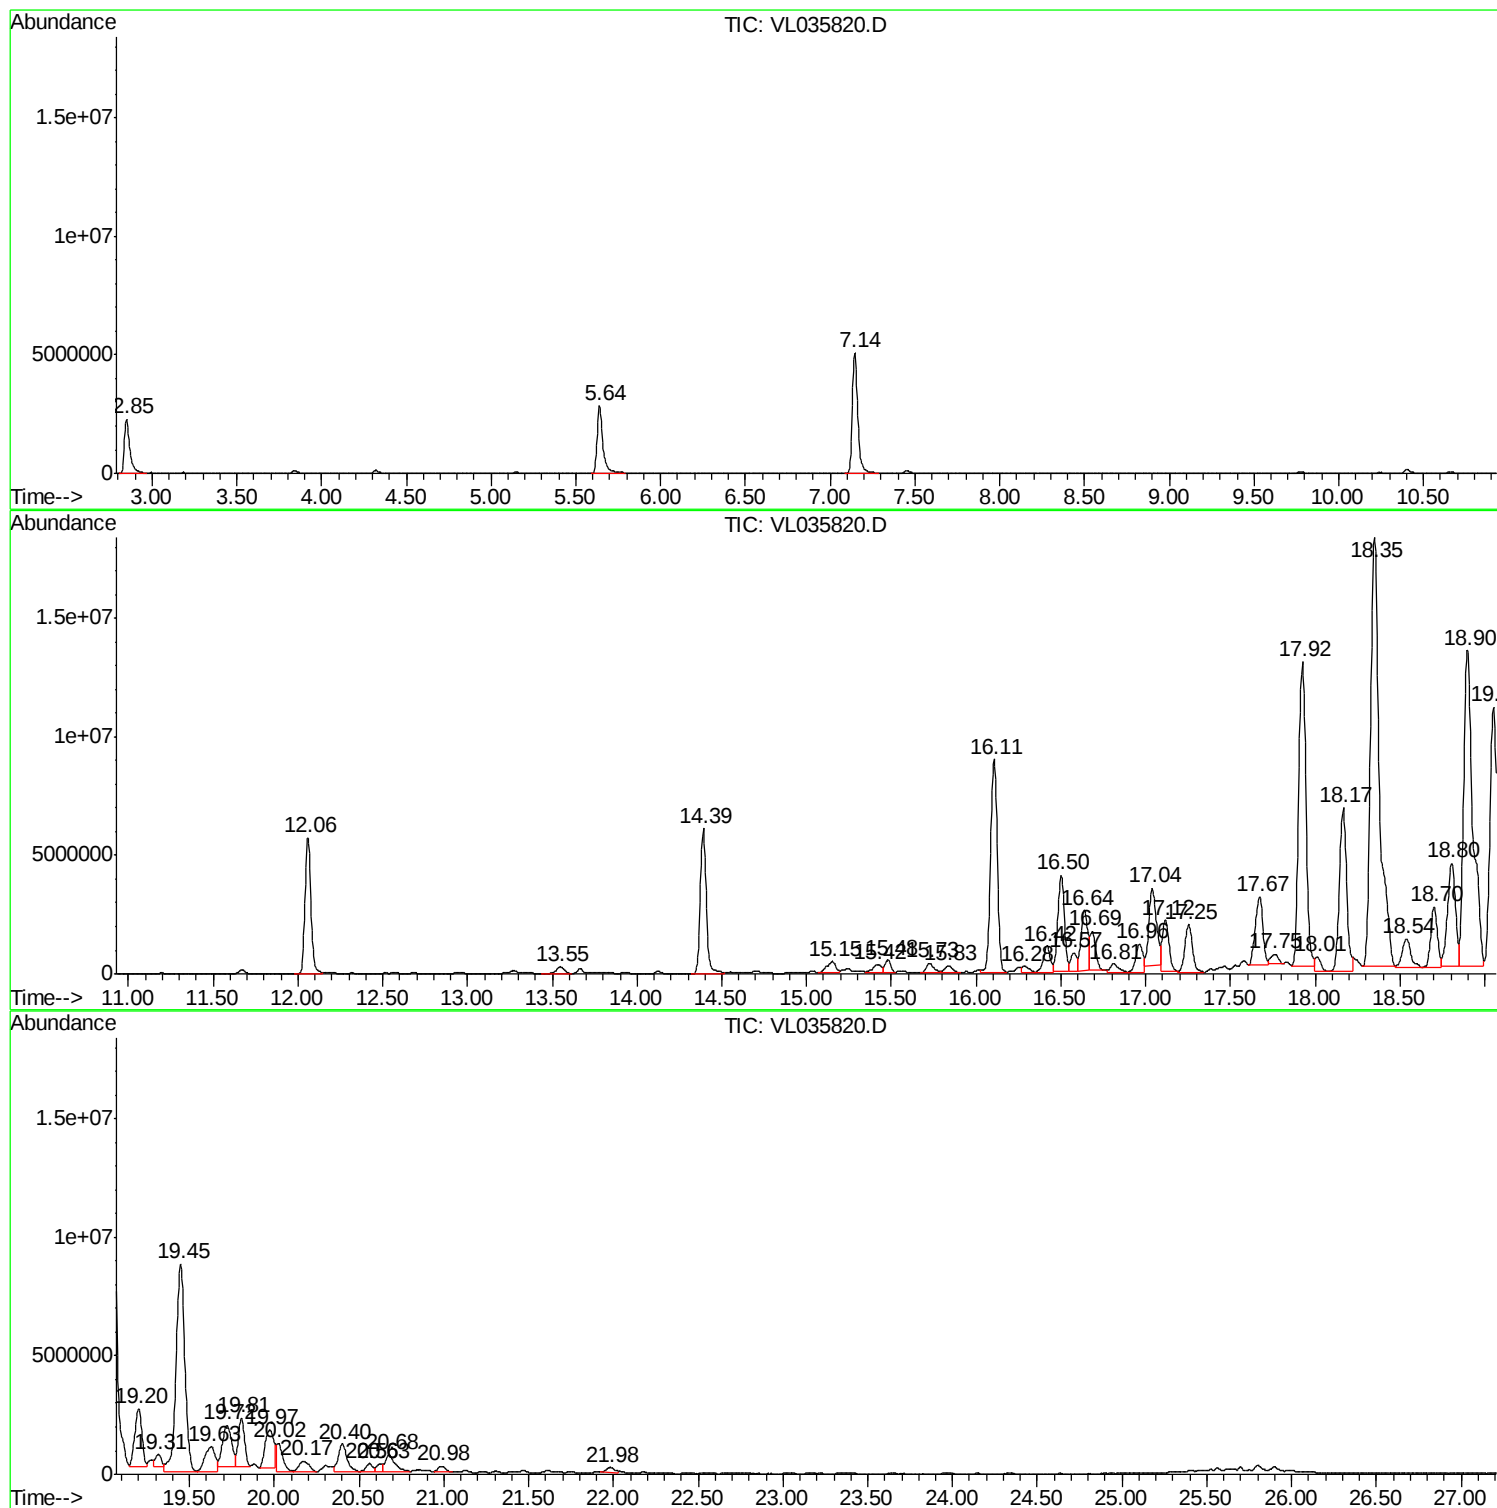

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL110320\
Data File : VL035820.D
Acq On : 4 Nov 2020 1:51
Operator : SY/AP
Sample : L4610-01 10X
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL110320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL110320\
Data File : VL035820.D
Acq On : 4 Nov 2020 1:51
Operator : SY/AP
Sample : L4610-01 10X
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL110320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc