

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL110320\
 Data File : VL035824.D
 Acq On : 4 Nov 2020 4:24
 Operator : SY/AP
 Sample : L4610-03 10X
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV3

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 3
 Start Thrs: 0.001
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.851	7	20	57	rBV	2273898	5030885	7.49%	1.063%
2	5.639	871	887	938	rBV	2769431	6411828	9.54%	1.355%
3	7.143	1336	1355	1399	rBV2	5014622	11164307	16.62%	2.359%
4	12.056	2864	2883	2912	rBV	5581157	13587855	20.22%	2.871%
5	13.548	3317	3347	3365	rBV6	299466	974408	1.45%	0.206%
6	14.391	3588	3609	3646	rBV	5934000	14688151	21.86%	3.104%
7	15.153	3819	3846	3860	rBV6	441834	1628820	2.42%	0.344%
8	15.410	3905	3926	3938	rBV4	295972	1019675	1.52%	0.215%
9	15.481	3938	3948	3962	rVB2	474864	1104187	1.64%	0.233%
10	15.722	4007	4023	4044	rBV6	383256	1199565	1.79%	0.253%
11	15.831	4044	4057	4079	rVB6	283012	843192	1.26%	0.178%
12	16.104	4115	4142	4166	rVB	8819031	24090921	35.86%	5.090%
13	16.413	4218	4238	4249	rBV2	1038441	2868725	4.27%	0.606%
14	16.500	4249	4265	4279	rVV2	3968450	10629677	15.82%	2.246%
15	16.574	4279	4288	4295	rVV3	735257	1777214	2.65%	0.376%
16	16.635	4295	4307	4317	rVV4	2497169	7007905	10.43%	1.481%
17	16.683	4317	4322	4349	rVV2	1577538	3685919	5.49%	0.779%
18	16.809	4349	4361	4387	rVB6	350303	1111577	1.65%	0.235%
19	16.963	4387	4409	4419	rBV2	1166911	3476061	5.17%	0.734%
20	17.037	4419	4432	4447	rVV5	3346051	11040296	16.43%	2.333%
21	17.114	4447	4456	4479	rVB2	2083092	5716571	8.51%	1.208%
22	17.249	4479	4498	4528	rVB6	1958857	5977818	8.90%	1.263%
23	17.577	4588	4600	4609	rVV3	373384	992781	1.48%	0.210%
24	17.667	4609	4628	4644	rVV4	3045689	9984714	14.86%	2.110%
25	17.757	4644	4656	4672	rVV5	620729	2420463	3.60%	0.511%
26	17.924	4688	4708	4730	rVV	12870626	39357077	58.58%	8.316%
27	18.011	4730	4735	4759	rVB2	662163	1470004	2.19%	0.311%
28	18.162	4759	4782	4817	rBV2	6792781	21804361	32.45%	4.607%
29	18.346	4817	4839	4879	rVV	18255799	67185724	100.00%	14.196%
30	18.535	4879	4898	4914	rVV4	1242953	4229538	6.30%	0.894%
31	18.699	4926	4949	4963	rVV2	2638739	7230705	10.76%	1.528%
32	18.805	4963	4982	4994	rVV4	4474877	14690241	21.87%	3.104%
33	18.895	4994	5010	5041	rVV	13577232	52470902	78.10%	11.087%
34	19.050	5041	5058	5087	rVV2	11293984	34172271	50.86%	7.220%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL110320\
Data File : VL035824.D
Acq On : 4 Nov 2020 4:24
Operator : SY/AP
Sample : L4610-03 10X
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV3

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 3 Min Area: 3 % of largest Peak
Start Thrs: 0.001 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Nov 04 02:40:06 2020

35	19.198	5087	5104	5118	rVV6	2601063	7697595	11.46%	1.626%
36	19.268	5118	5126	5131	rVV4	345636	719078	1.07%	0.152%
37	19.317	5131	5141	5151	rVV3	589355	1486463	2.21%	0.314%
38	19.445	5151	5181	5210	rVB4	9156255	33012906	49.14%	6.975%
39	19.625	5210	5237	5249	rBV2	1127754	4712505	7.01%	0.996%
40	19.718	5249	5266	5281	rVV5	1907231	7143164	10.63%	1.509%
41	19.805	5281	5293	5308	rVV2	2198117	5700754	8.49%	1.205%
42	19.972	5325	5345	5356	rBV6	1803821	6571714	9.78%	1.389%
43	20.017	5356	5359	5386	rVB3	1317957	3192347	4.75%	0.675%
44	20.165	5386	5405	5429	rVB4	500790	2032449	3.03%	0.429%
45	20.400	5461	5478	5508	rVB3	1364408	4720733	7.03%	0.997%
46	20.558	5508	5527	5536	rBV4	397716	1028343	1.53%	0.217%
47	20.625	5536	5548	5552	rVV7	321096	778791	1.16%	0.165%
48	20.673	5552	5563	5589	rVB3	745301	2536543	3.78%	0.536%
49	21.979	5951	5969	5984	rBV5	265215	894066	1.33%	0.189%


Sum of corrected areas: 473271789

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL110320\
Data File : VL035824.D
Acq On : 4 Nov 2020 4:24
Operator : SY/AP
Sample : L4610-03 10X
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampled :
SV3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

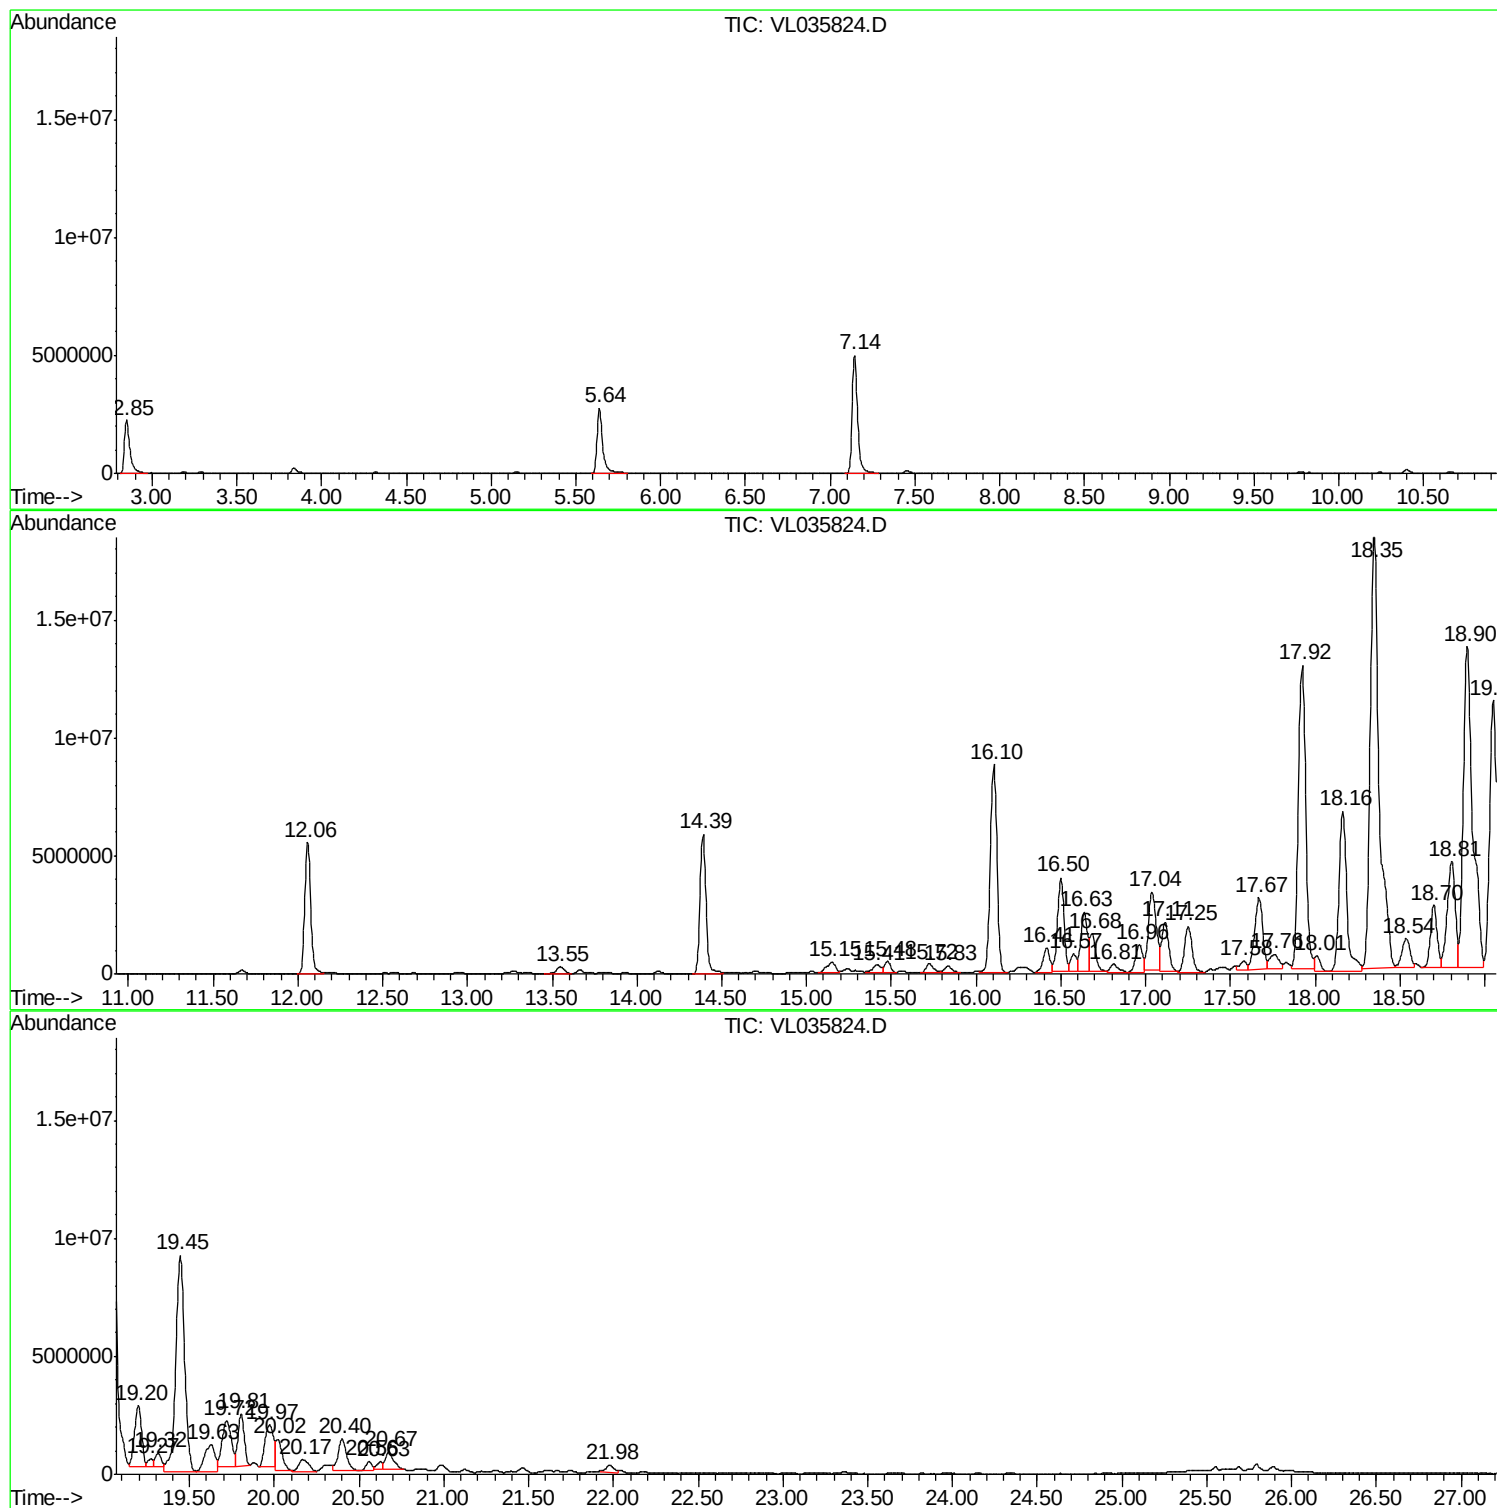

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL110320\
Data File : VL035824.D
Acq On : 4 Nov 2020 4:24
Operator : SY/AP
Sample : L4610-03 10X
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL110320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL110320\
Data File : VL035824.D
Acq On : 4 Nov 2020 4:24
Operator : SY/AP
Sample : L4610-03 10X
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL110320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc