


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL110320\
 Data File : VL035798.D
 Acq On : 3 Nov 2020 9:52
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL110320AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Nov 04 02:40:06 2020
 Last Update : Wed Nov 04 02:40:06 2020

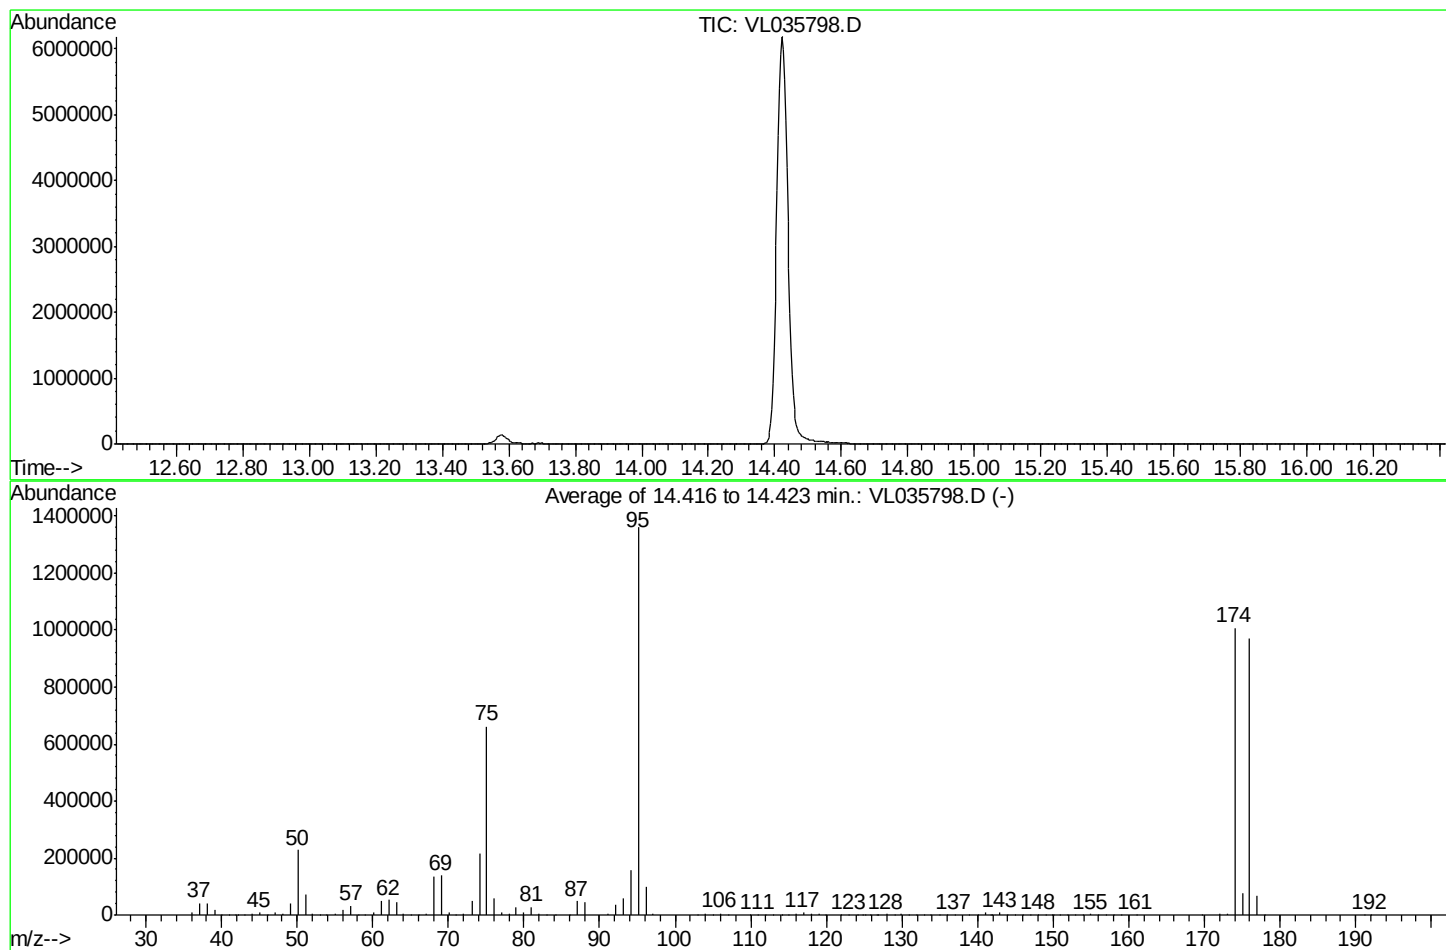

AutoFind: Scans 3617, 3618, 3619; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	16.8	228778	PASS
75	95	30	66	48.6	661888	PASS
95	95	100	100	100.0	1360896	PASS
96	95	5	9	7.3	99082	PASS
173	174	0.00	2	0.5	5489	PASS
174	95	50	120	74.1	1008917	PASS
175	174	4	9	7.5	75181	PASS
176	174	93	101	96.1	969408	PASS
177	176	5	9	6.8	65626	PASS