
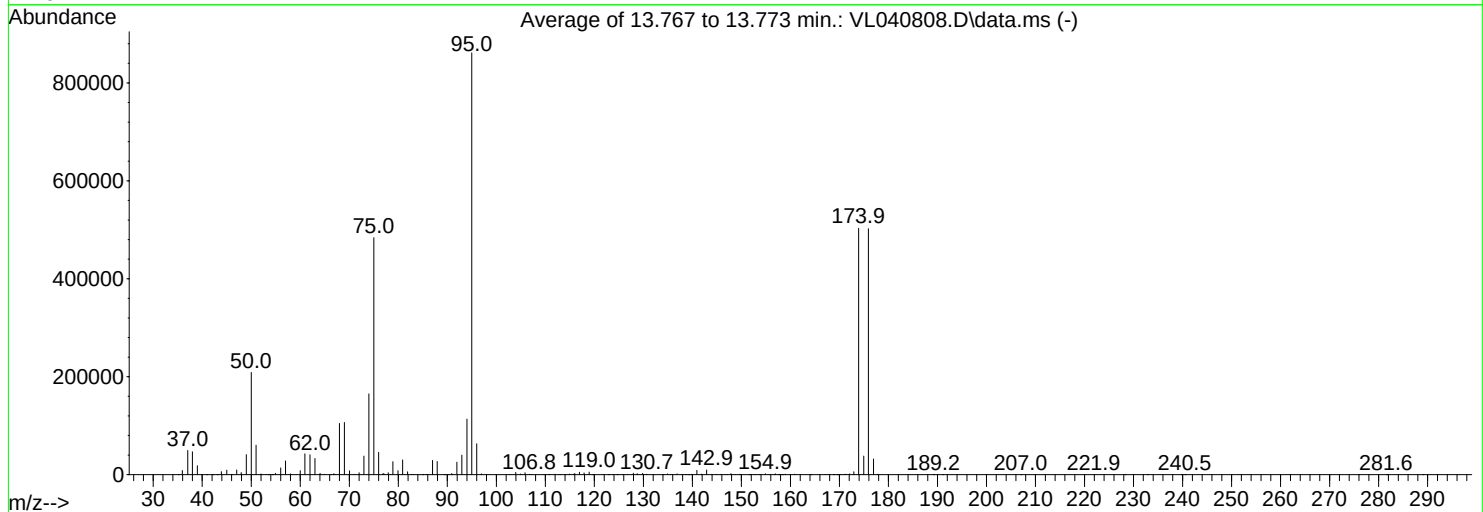


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110823\
Data File : VL040808.D
Acq On : 8 Nov 2023 12:30
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101123AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Nov 09 00:25:02 2023

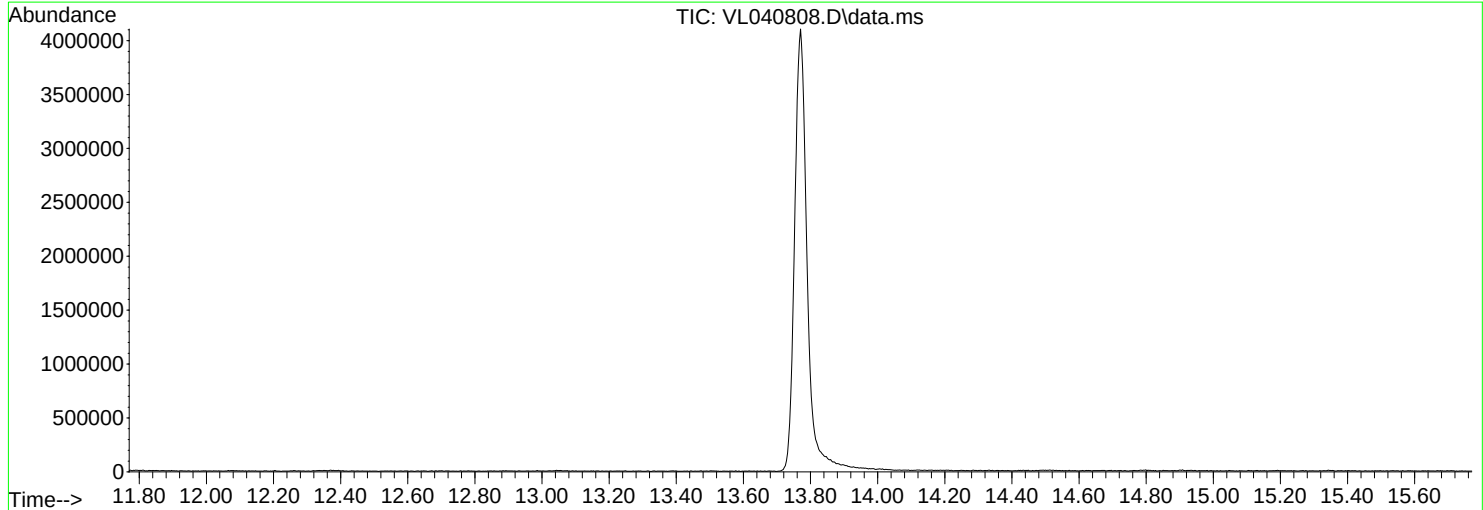

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.2	208768	PASS
75	95	30	66	56.2	483996	PASS
95	95	100	100	100.0	861397	PASS
96	95	5	9	7.3	62923	PASS
173	174	0.00	2	1.2	6077	PASS
174	95	50	120	58.4	503083	PASS
175	174	4	9	7.5	37920	PASS
176	174	93	101	99.8	502293	PASS
177	176	5	9	6.4	32200	PASS

Average of 13.767 to 13.773 min.: VL040808.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	55	45.00	9055	53.50	83	64.95	80
35.95	8422	45.95	547	54.30	54	66.30	20
37.05	49224	46.20	208	54.95	2671	66.85	203
38.00	46592	47.05	9632	56.00	13906	67.10	48
39.00	18468	47.95	4148	57.00	28088	68.00	104704
39.90	305	49.00	40763	58.05	1683	69.00	106528
40.00	245	50.00	208768	60.00	8137	70.05	8003
40.90	130	51.00	60165	60.95	42539	71.00	553
42.20	93	51.85	1124	62.00	40589	72.00	3889
43.05	177	52.10	881	63.00	33023	73.00	37811
43.90	6086	53.00	193	64.05	2667	74.00	164992

Average of 13.767 to 13.773 min.: VL040808.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.00	483996	85.00	81	94.00	113299	110.00	435
76.00	45605	85.70	197	95.00	861397	110.70	347
76.90	2736	86.00	222	96.00	62923	110.90	622
77.10	1234	87.00	28947	96.95	1822	111.95	981
77.95	3961	87.95	26725	102.80	362	112.75	470
78.90	26376	89.40	100	103.95	4576	113.05	490
79.95	8245	90.30	259	104.95	1458	114.00	134
80.90	30069	90.85	1993	105.85	3969	114.90	1366
81.90	5805	91.10	923	106.75	807	115.70	872
82.75	585	91.95	25507	107.20	283	116.00	2154
83.10	212	92.95	39939	109.70	223	116.95	4988

Average of 13.767 to 13.773 min.: VL040808.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.90	3671	129.85	2636	139.20	80	147.85	1845
118.95	5160	130.70	1095	139.85	730	148.85	328
119.70	119	132.00	69	140.90	8894	149.65	655
121.80	603	134.00	125	141.85	1126	149.90	322
122.90	111	134.95	1774	142.90	9657	151.60	164
123.80	712	135.60	214	143.85	507	151.90	511
124.65	138	135.95	308	144.10	281	152.75	484
125.80	801	136.85	1671	144.90	754	153.00	193
126.75	196	137.85	219	145.80	798	153.70	203
127.95	2900	138.60	232	146.70	435	153.90	270
128.75	1927	138.90	253	147.10	466	154.90	1940

Average of 13.767 to 13.773 min.: VL040808.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.75	248	168.80	139	174.95	37920	239.80	52
156.70	392	169.00	392	175.90	502293	240.50	154
156.95	1625	169.50	82	176.95	32200	275.90	52
157.60	74	169.80	272	177.80	809	281.60	89
158.10	327	170.20	401	178.00	551	289.00	53
158.40	144	170.70	242	189.20	130		
158.95	835	171.15	848	191.10	118		
160.90	1121	171.40	664	207.00	93		
164.20	167	172.10	1574	221.90	74		
167.10	201	172.95	6077	228.30	53		
167.85	492	173.90	503083	232.80	142		