
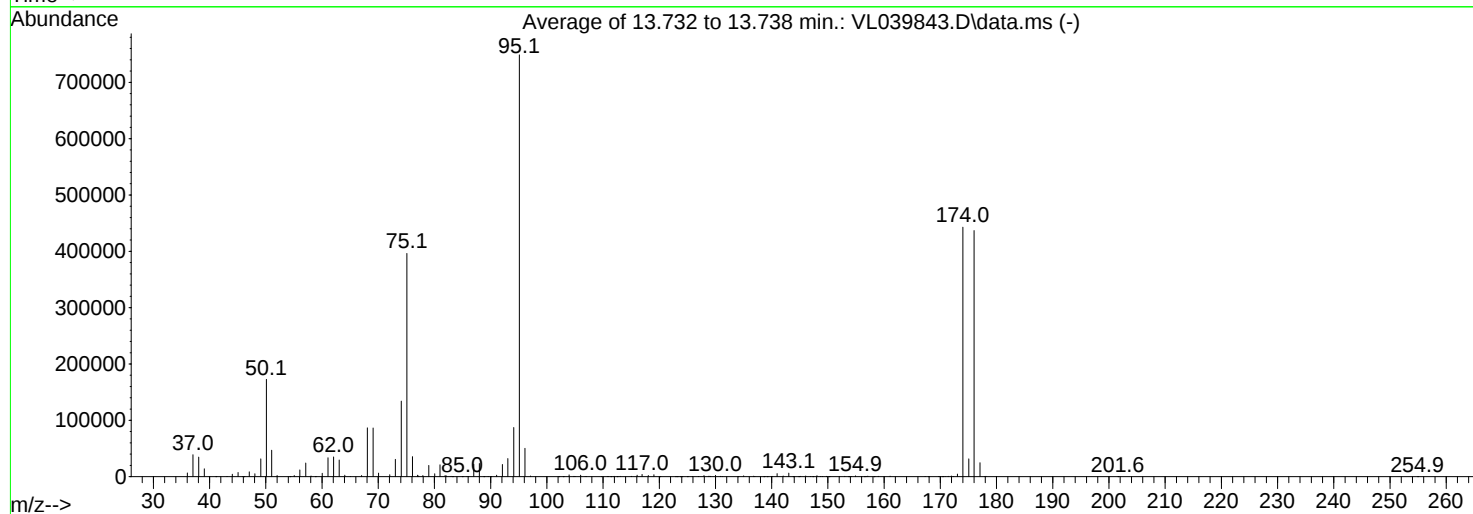


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110922\
 Data File : VL039843.D
 Acq On : 9 Nov 2022 11:00
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL110222AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Thu Nov 03 09:27:12 2022

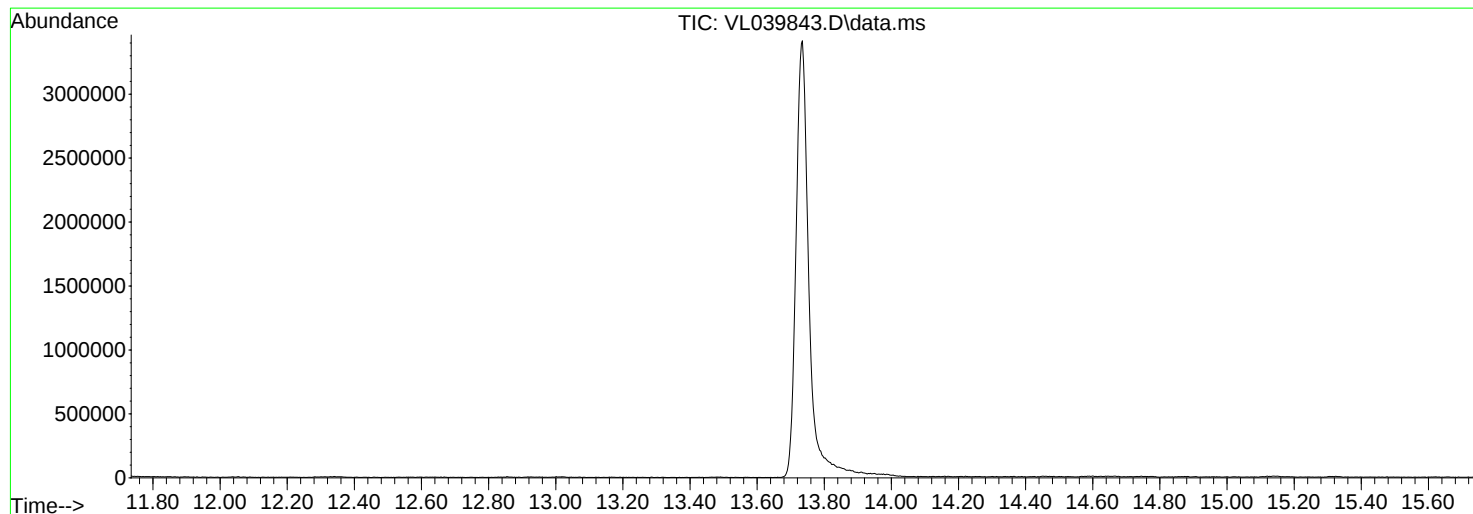

AutoFind: Scans 3461, 3462, 3463; Background Corrected with Scan 3435

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.1	172608	PASS
75	95	30	66	52.9	396288	PASS
95	95	100	100	100.0	748800	PASS
96	95	5	9	6.7	50261	PASS
173	174	0.00	2	1.0	4476	PASS
174	95	50	120	59.2	442944	PASS
175	174	4	9	7.1	31589	PASS
176	174	93	101	98.6	436736	PASS
177	176	5	9	5.7	24843	PASS

Average of 13.732 to 13.738 min.: VL039843.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6545	47.05	8625	58.80	152	72.05	337
37.05	39027	48.05	5043	60.05	5896	73.05	3068
38.05	34568	49.10	31451	61.05	33459	74.10	13408
39.05	13877	50.10	172608	62.05	34984	75.10	39628
40.00	214	51.05	46949	63.05	29643	76.10	35491
41.10	115	52.00	1885	64.05	2433	77.00	2621
43.10	441	54.30	89	65.05	203	77.20	1281
44.05	4232	55.05	2124	67.05	2065	77.95	1902
45.05	7375	56.05	11832	68.05	86733	79.00	19877
45.90	407	57.10	24093	69.10	86285	80.05	5008
46.10	158	58.05	1220	70.05	6273	81.00	21141

Average of 13.732 to 13.738 min.: VL039843.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	1884	90.00	55	104.80	688	113.05	572
82.10	1313	91.05	2480	105.00	276	115.05	455
82.95	513	92.10	21627	106.00	2523	116.05	2552
83.20	128	93.05	32235	106.80	214	116.95	3927
84.95	118	94.10	87267	107.00	418	118.05	1909
85.80	310	95.10	748800	109.75	305	119.05	3374
86.05	385	96.10	50261	110.75	252	120.10	69
87.00	22299	97.10	1162	110.95	382	122.90	145
88.00	23339	102.10	75	111.40	148	123.20	116
88.80	132	102.90	82	111.95	508	123.70	93
89.55	206	103.95	3028	112.50	59	124.00	152

Average of 13.732 to 13.738 min.: VL039843.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.00	140	136.80	777	144.80	60	153.00	625
125.90	250	137.00	219	145.10	550	153.70	111
127.00	234	138.60	71	146.05	1096	154.15	241
127.95	2119	138.80	356	146.90	247	154.90	1494
128.85	950	139.20	143	147.30	123	156.00	385
129.10	484	140.05	577	148.05	1632	156.50	152
130.00	2233	140.95	5525	148.70	221	156.90	375
130.90	515	142.05	1095	149.05	232	157.10	837
131.20	433	143.05	6190	149.75	590	158.20	53
134.00	73	143.80	107	150.20	128	158.95	701
135.00	1336	144.05	337	152.05	287	161.05	934

Average of 13.732 to 13.738 min.: VL039843.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
167.30	174	175.05	31589				
167.90	130	176.00	436736				
169.70	189	177.05	24843				
169.90	244	177.90	428				
170.40	159	178.10	693				
170.85	417	201.60	72				
171.40	584	254.90	106				
171.95	1293						
172.30	445						
173.05	4476						
174.00	442944						