

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL111020\
 Data File : VL035899.D
 Acq On : 10 Nov 2020 21:51
 Operator : SY/AP
 Sample : OC102920 CAN 10604
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC102920 CAN 10604

Quant Time: Nov 11 09:39:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020
 QLast Update : Wed Nov 04 02:40:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.65	49	1051034	10.00	ppbv	-0.01
33) 1,4-Difluorobenzene	7.16	114	3876439	10.00	ppbv	-0.02
55) Chlorobenzene-d5	12.08	117	3634973	10.00	ppbv	-0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.41	95	2640782	10.23	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.30%


Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL111020\
Data File : VL035899.D
Acq On : 10 Nov 2020 21:51
Operator : SY/AP
Sample : OC102920 CAN 10604
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC102920 CAN 10604

Quant Time: Nov 11 09:39:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Nov 04 02:40:06 2020
QLast Update : Wed Nov 04 02:40:06 2020
Response via : Initial Calibration

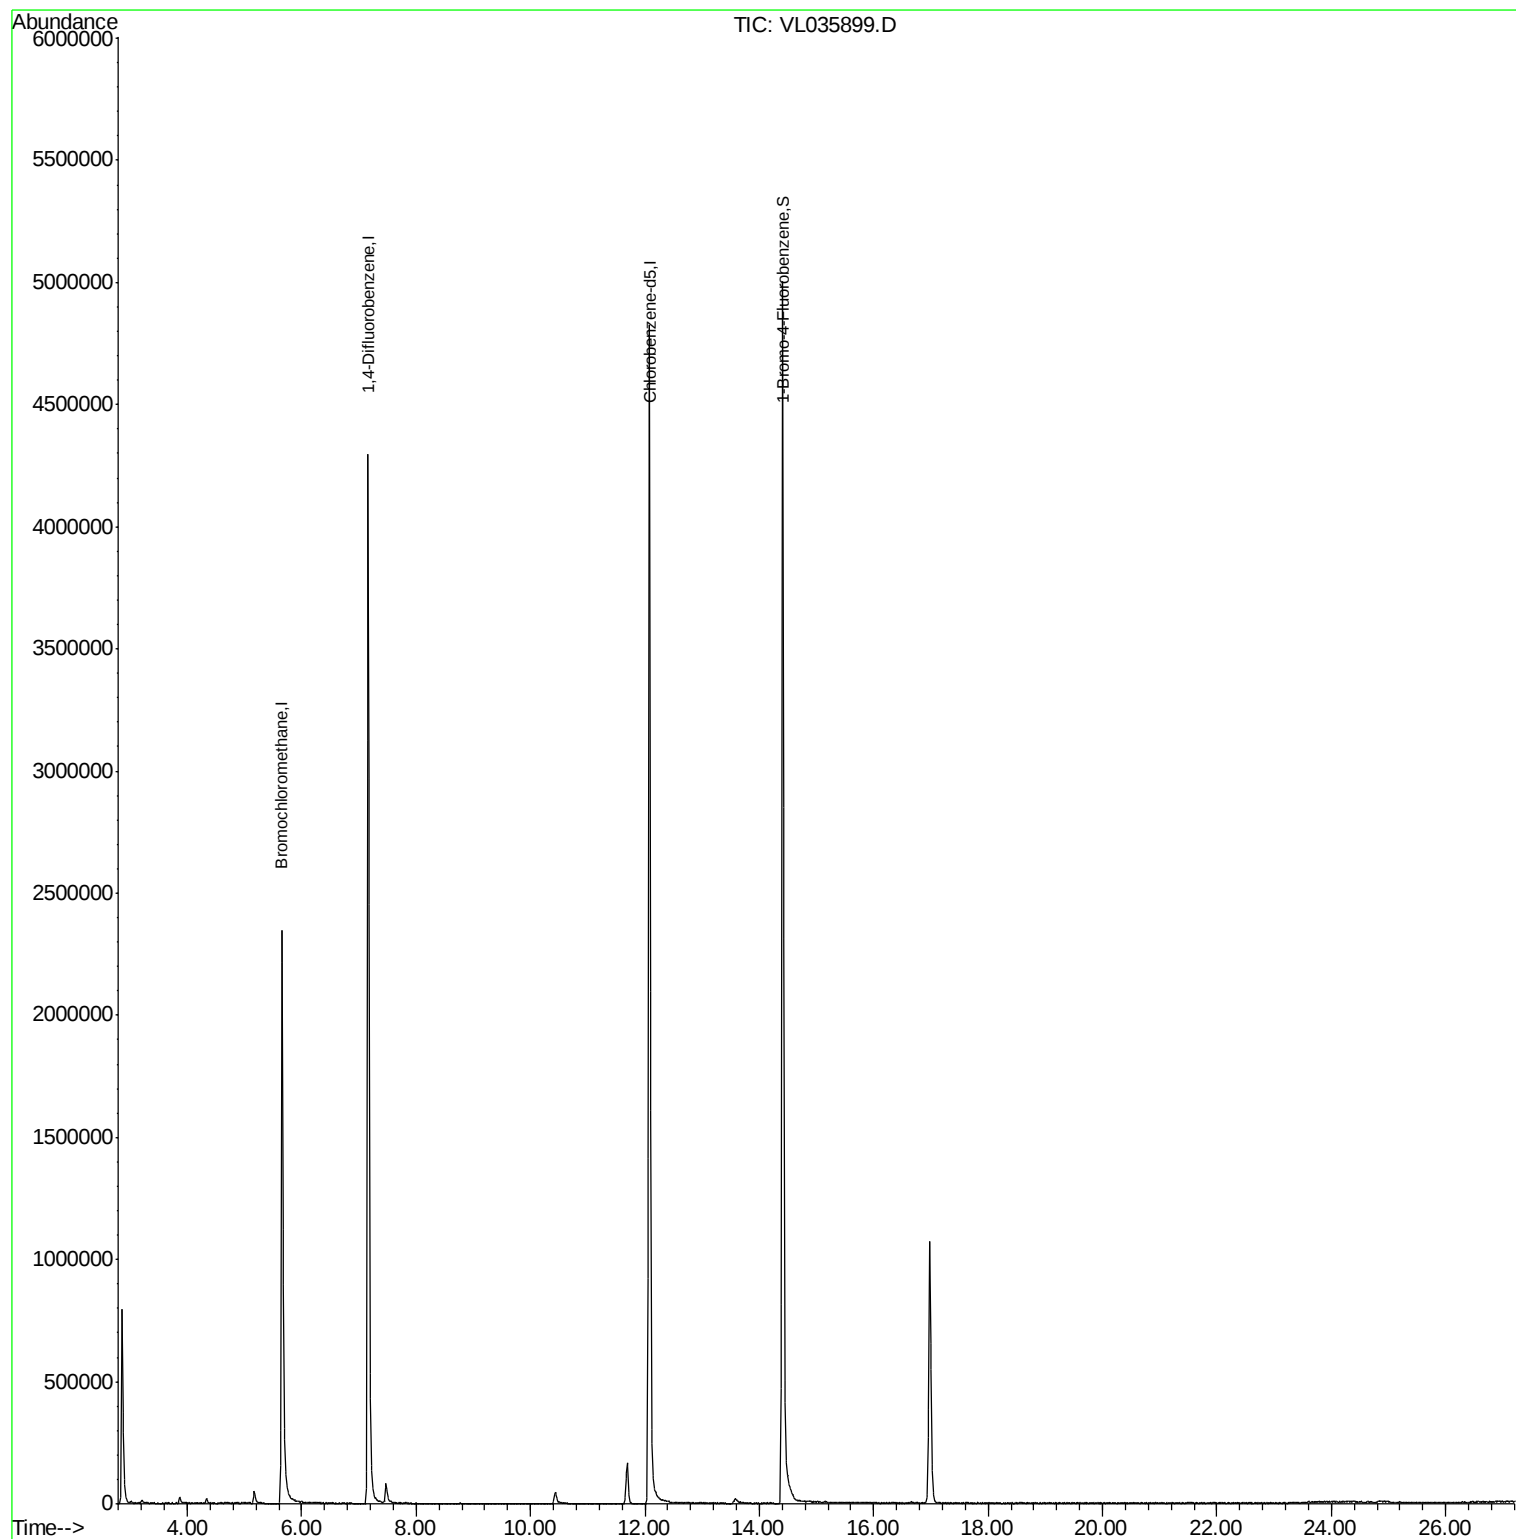



#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.65 min Scan# 892

Delta R.T. -0.01 min

Lab File: VL035899.D

Acq: 10 Nov 2020 21:51

Instrument :

MSVOA_L

ClientSampleId :

QC102920 CAN 10604


Tot Ion: 49 Resp: 1051034

Ion Ratio Lower Upper

49 100

128 81.3 41.5 124.6

130 104.7 53.7 161.1



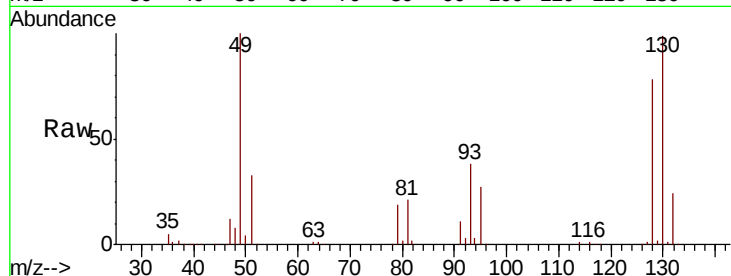


Abundance

Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

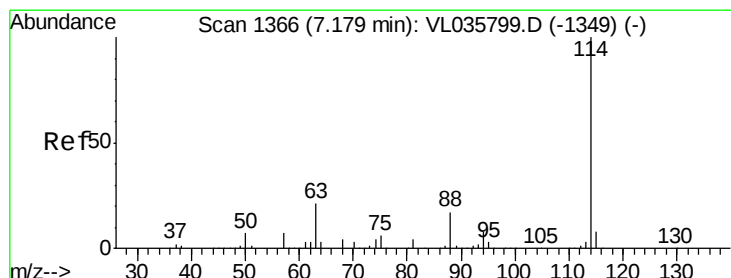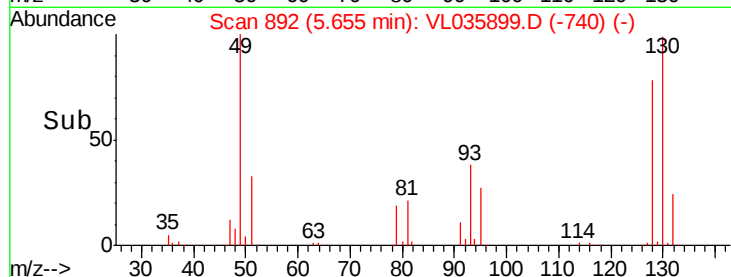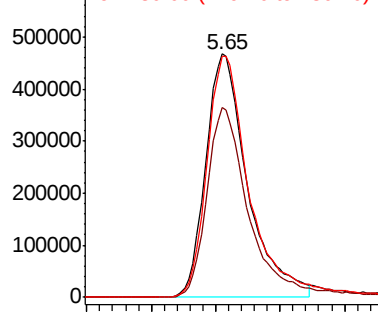

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.16 min Scan# 1361

Delta R.T. -0.02 min

Lab File: VL035899.D

Acq: 10 Nov 2020 21:51


Tgt Ion: 114 Resp: 3876439

Ion Ratio Lower Upper

114 100

63 20.7 16.1 24.1

88 17.4 13.7 20.5


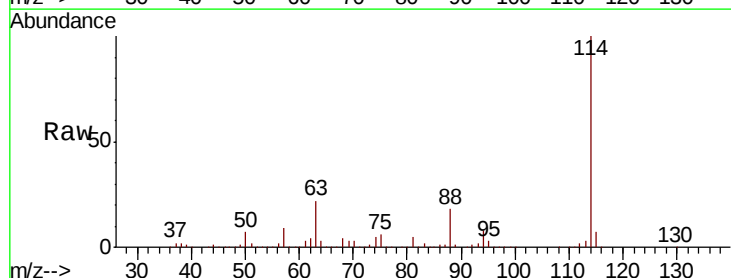



Abundance

Ion 114.10 (113.80 to 114.80): V

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

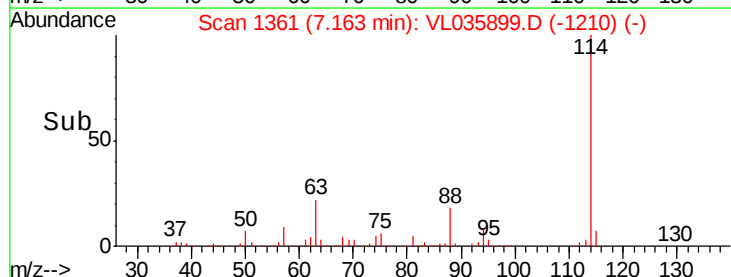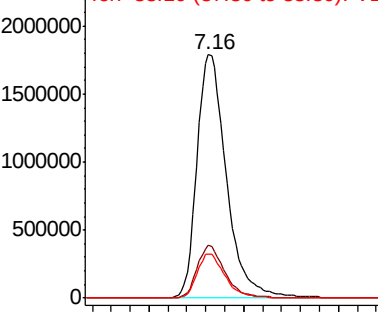


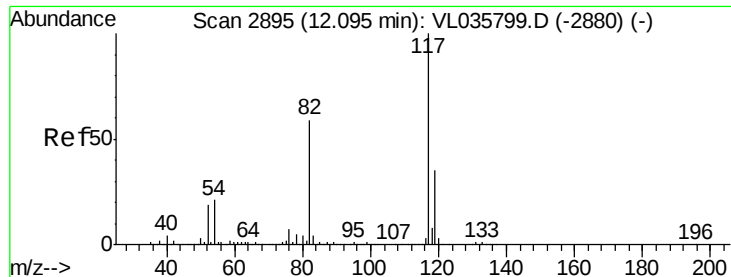




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.08 min Scan# 2889
Delta R.T. -0.02 min
Lab File: VL035899.D
Acq: 10 Nov 2020 21:51

Instrument :
MSVOA_L
ClientSampleId :
QC102920 CAN 10604

Tot Ion:117 Resp: 3634973
Ion Ratio Lower Upper
117 100
82 61.3 50.6 76.0
119 34.3 52.6 78.8#

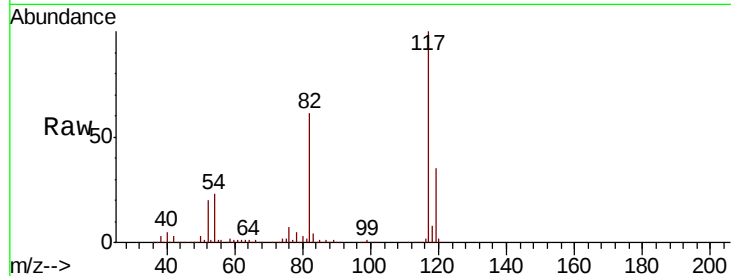


Abundance Ion 117.10 (116.80 to 117.80): V
Ion 82.10 (81.80 to 82.80): VL0
Ion 119.10 (118.80 to 119.80): V

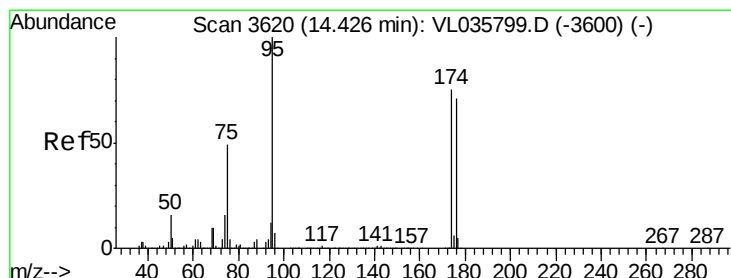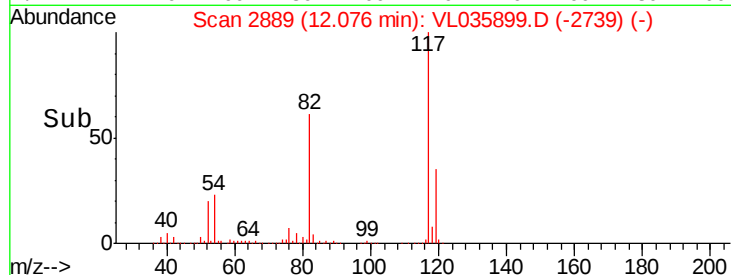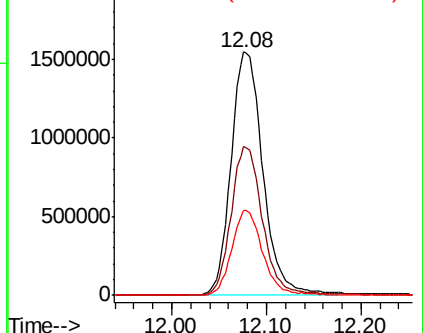

#68
1-Bromo-4-Fluorobenzene
Concen: 10.225 ppbv
RT: 14.41 min Scan# 3614
Delta R.T. -0.02 min
Lab File: VL035899.D
Acq: 10 Nov 2020 21:51

Tgt Ion: 95 Resp: 2640782
Ion Ratio Lower Upper
95 100
174 75.2 59.8 89.6
175 5.2 4.3 6.5

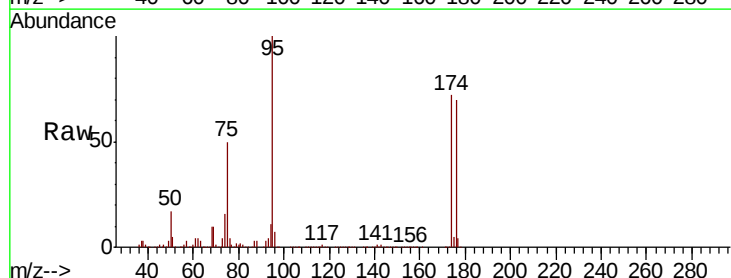

Abundance Ion 95.10 (94.80 to 95.80): VL0
Ion 174.00 (173.70 to 174.70): V
Ion 175.00 (174.70 to 175.70): V

