
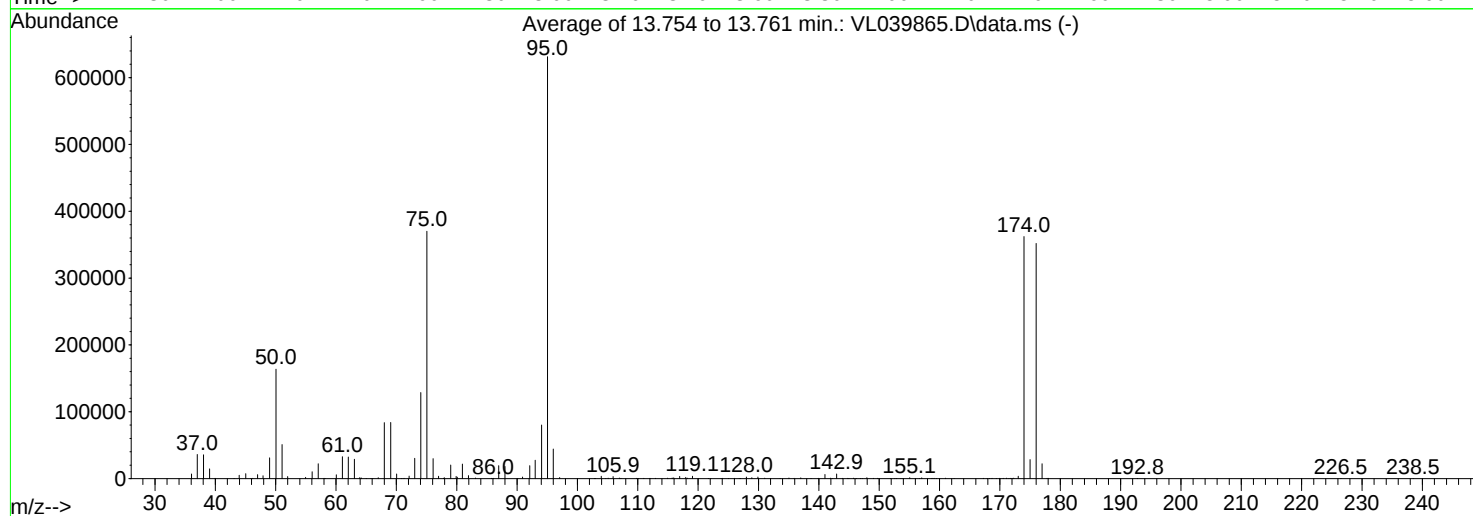


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL111022\
 Data File : VL039865.D
 Acq On : 10 Nov 2022 12:26
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL110222AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Thu Nov 03 09:27:12 2022

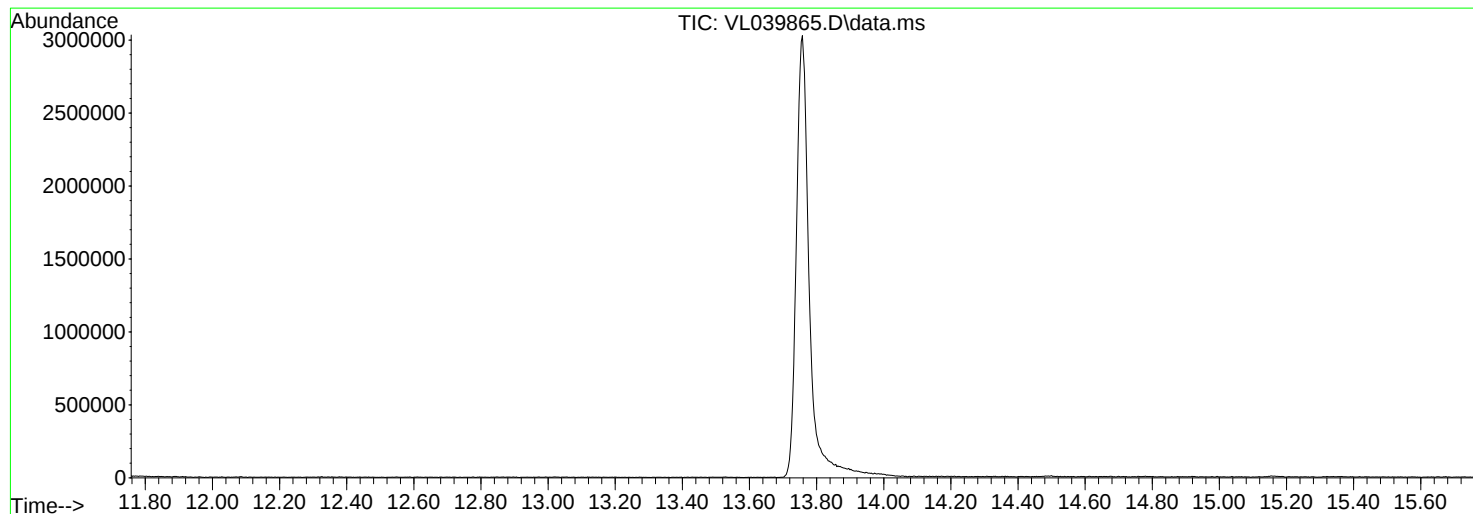

AutoFind: Scans 3468, 3469, 3470; Background Corrected with Scan 3444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.9	163733	PASS
75	95	30	66	58.6	370048	PASS
95	95	100	100	100.0	631253	PASS
96	95	5	9	7.0	44117	PASS
173	174	0.00	2	1.0	3591	PASS
174	95	50	120	57.4	362261	PASS
175	174	4	9	7.8	28288	PASS
176	174	93	101	97.2	352021	PASS
177	176	5	9	6.3	22267	PASS

Average of 13.754 to 13.761 min.: VL039865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6735	47.90	4128	61.05	32592	70.05	6844
37.00	35976	49.00	31061	62.05	32195	70.90	64
38.05	35693	50.05	163733	63.05	28808	71.25	358
39.05	14474	51.05	50955	63.95	1677	72.10	3775
39.95	504	52.00	2923	64.20	831	73.05	30333
43.10	218	54.95	1937	65.00	150	74.05	128787
43.95	4939	56.05	10317	65.80	171	75.05	370048
45.05	7272	57.05	22235	66.10	100	76.10	29765
45.90	193	58.00	449	67.00	1437	77.00	3564
46.20	390	58.20	233	68.00	83600	77.80	443
47.00	6002	60.05	5738	69.05	83888	77.95	1404

Average of 13.754 to 13.761 min.: VL039865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.00	20128	90.90	2369	105.10	731	115.95	1116
79.90	3208	92.10	19341	105.90	2948	116.95	3181
80.10	2147	93.00	27435	106.95	797	117.95	1820
80.95	21595	94.05	80000	107.20	428	118.20	597
81.95	4486	95.05	631253	109.80	271	119.05	3458
83.10	841	96.00	44117	110.10	176	120.10	136
85.80	368	97.05	1627	111.00	511	121.70	67
86.05	369	102.80	240	112.00	481	122.10	57
86.95	19339	103.00	96	112.95	486	123.80	179
88.00	18112	103.95	3363	114.95	573	124.05	262
90.10	200	104.70	193	115.70	750	125.05	183

Average of 13.754 to 13.761 min.: VL039865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.00	363	137.00	1025	146.20	119	155.05	1345
126.80	60	138.70	103	146.90	58	156.00	112
127.05	163	139.90	382	147.20	116	156.70	113
128.00	2431	141.00	6161	147.95	1449	157.05	1155
128.90	1471	141.95	543	149.05	314	158.75	333
129.90	2337	142.20	225	149.75	268	159.10	387
131.05	664	142.95	6890	151.90	180	159.50	62
132.00	98	143.90	451	152.60	133	161.00	639
133.60	118	144.80	347	152.90	91	162.40	66
135.05	790	145.00	141	153.60	58	167.25	266
135.90	311	145.75	600	153.95	151	167.90	54

Average of 13.754 to 13.761 min.: VL039865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
168.30	150	174.00	362261				
168.70	263	175.00	28288				
169.40	123	176.00	352021				
169.95	505	177.00	22267				
170.55	491	177.80	281				
171.10	700	178.05	443				
171.50	169	192.80	77				
171.80	507	226.50	81				
172.00	321	238.50	127				
172.30	536						
173.05	3591						