


Data Path : W:\HPCHEM1\MSVOA L\Data\VL111115\
Data File : VL026359.D
Acq On : 11 Nov 2015 9:57
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL102915AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Oct 29 14:29:54 2015
Last Update : Thu Oct 29 14:29:54 2015

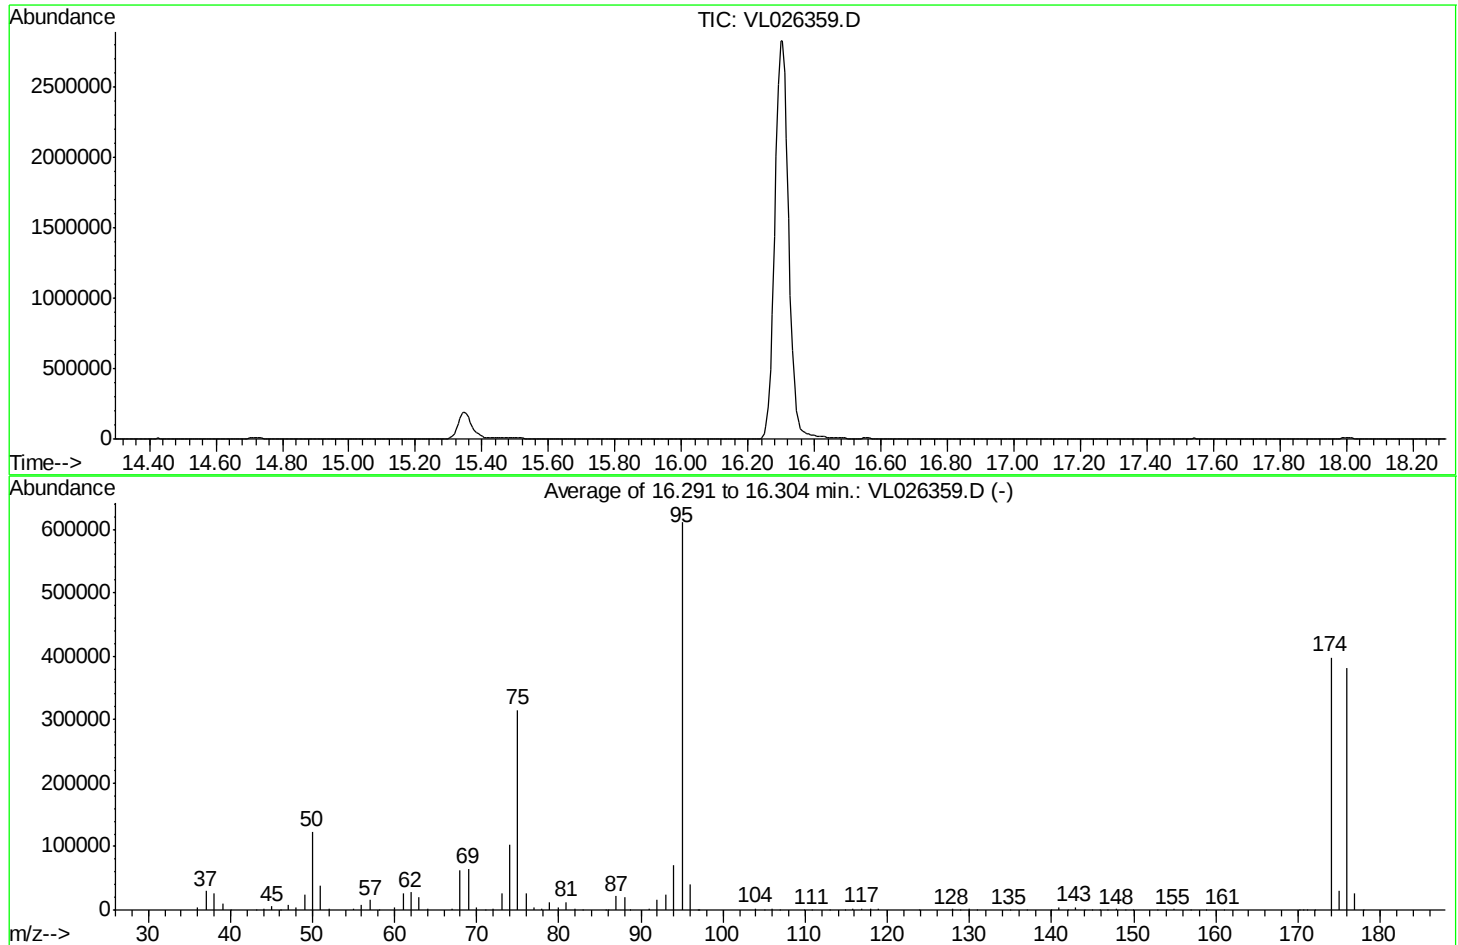

AutoFind: Scans 2166, 2167, 2168; Background Corrected with Scan 2151

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.3	123805	PASS
75	95	30	66	51.7	315669	PASS
95	95	100	100	100.0	610986	PASS
96	95	5	9	6.6	40584	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	65.2	398336	PASS
175	174	4	9	7.7	30600	PASS
176	174	93	101	95.7	381162	PASS
177	176	5	9	6.7	25400	PASS