
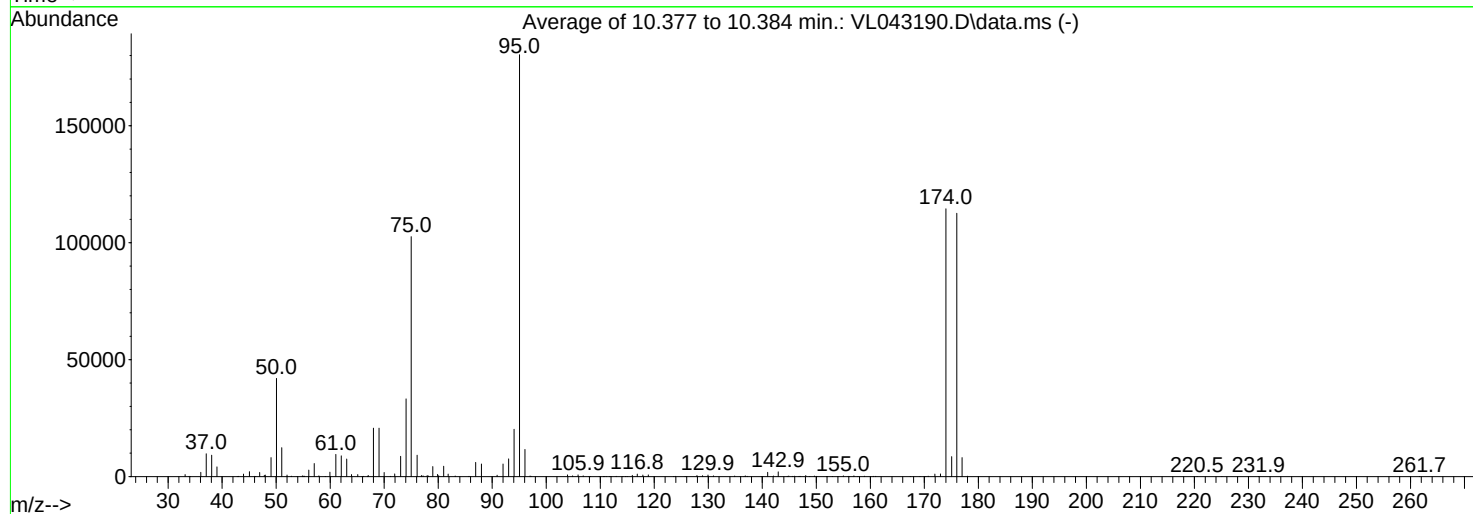


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL111325\
Data File : VL043190.D
Acq On : 13 Nov 2025 07:50
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Oct 15 02:12:58 2025

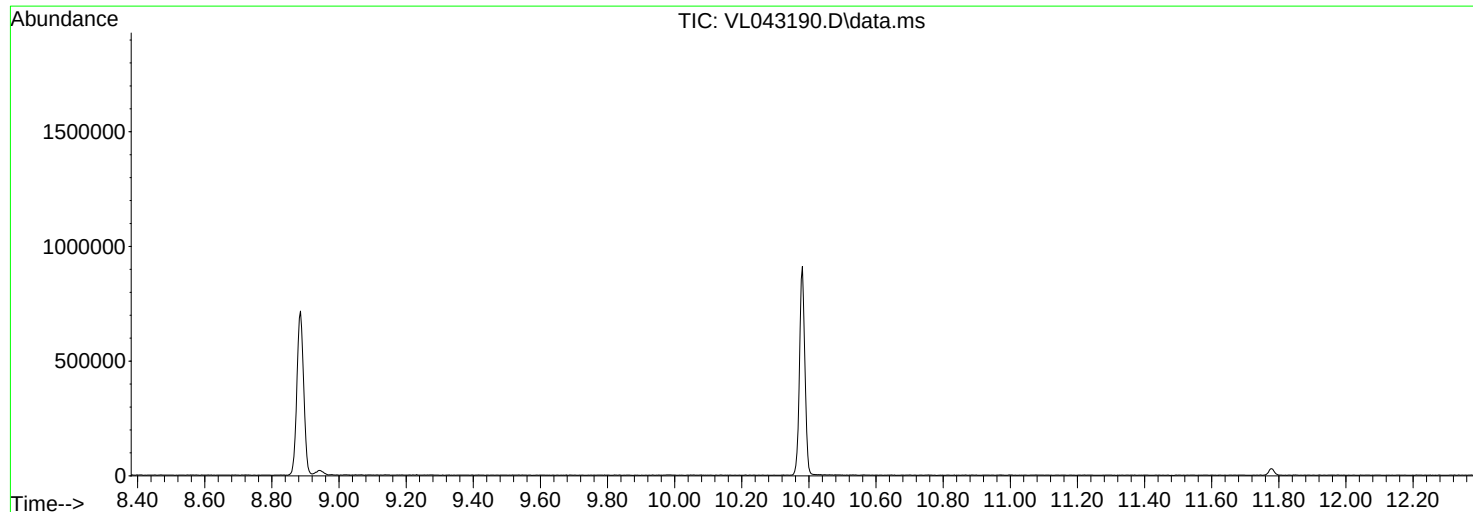

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.3	41979	PASS
75	95	30	66	56.9	102581	PASS
95	95	100	100	100.0	180352	PASS
96	95	5	9	6.4	11615	PASS
173	174	0.00	2	1.0	1106	PASS
174	95	50	120	63.5	114525	PASS
175	174	4	9	7.5	8536	PASS
176	174	93	101	98.3	112568	PASS
177	176	5	9	7.2	8084	PASS

Average of 10.377 to 10.384 min.: VL043190.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	856	46.00	99	54.85	327	63.95	889
33.90	110	46.20	41	55.00	181	65.10	889
34.10	31	46.95	1736	55.20	170	65.90	37
36.05	1842	47.80	512	56.05	2796	66.15	90
37.05	9770	48.00	651	57.05	5570	66.90	152
38.05	9156	49.05	8102	57.90	289	67.05	420
39.05	4163	50.05	41979	59.10	18	68.00	20709
42.80	45	51.05	12360	59.95	1904	69.05	20704
43.05	90	52.00	654	61.05	9495	70.00	1780
43.95	1095	52.80	151	62.05	8891	71.15	102
45.05	2120	53.90	18	63.05	7496	71.95	1155

Average of 10.377 to 10.384 min.: VL043190.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.05	8681	81.00	4419	96.05	11615	110.80	41
74.05	33251	81.85	1082	97.00	249	111.10	63
75.00	102581	83.15	232	97.20	88	111.75	57
76.10	9115	85.70	137	103.95	692	112.00	68
76.90	472	86.95	6093	104.90	336	112.95	134
77.20	286	88.00	5360	105.90	694	114.20	44
77.95	441	90.90	564	106.85	293	114.70	28
78.20	250	92.00	5355	107.90	21	115.00	44
79.00	4274	93.05	7592	108.20	39	115.95	509
79.90	914	94.05	20227	109.80	23	116.85	1080
80.10	401	95.05	180352	110.60	44	117.90	634

Average of 10.377 to 10.384 min.: VL043190.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.90	738	136.60	33	146.00	163	155.00	338
123.60	17	136.85	305	146.80	77	155.90	108
123.90	102	137.20	121	147.00	121	156.10	41
125.70	17	139.80	38	148.05	475	156.95	332
126.00	59	140.10	47	148.80	49	157.70	47
127.90	463	141.00	1819	149.65	251	158.90	165
128.95	415	142.05	215	150.10	123	160.55	86
129.95	626	142.95	1999	151.90	18	161.00	105
130.95	282	144.60	81	152.05	70	167.40	17
134.90	273	144.90	260	153.00	19	169.20	19
135.90	39	145.65	131	154.00	30	170.00	46

Average of 10.377 to 10.384 min.: VL043190.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.30	25	231.90	51				
170.70	164	261.70	25				
171.95	1061						
173.00	1106						
174.00	114525						
175.05	8536						
176.00	112568						
177.00	8084						
177.95	203						
220.50	18						
225.10	23						