


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL111423\
 Data File : VL040843.D
 Acq On : 14 Nov 2023 9:01
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111323AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Nov 20 03:50:24 2023

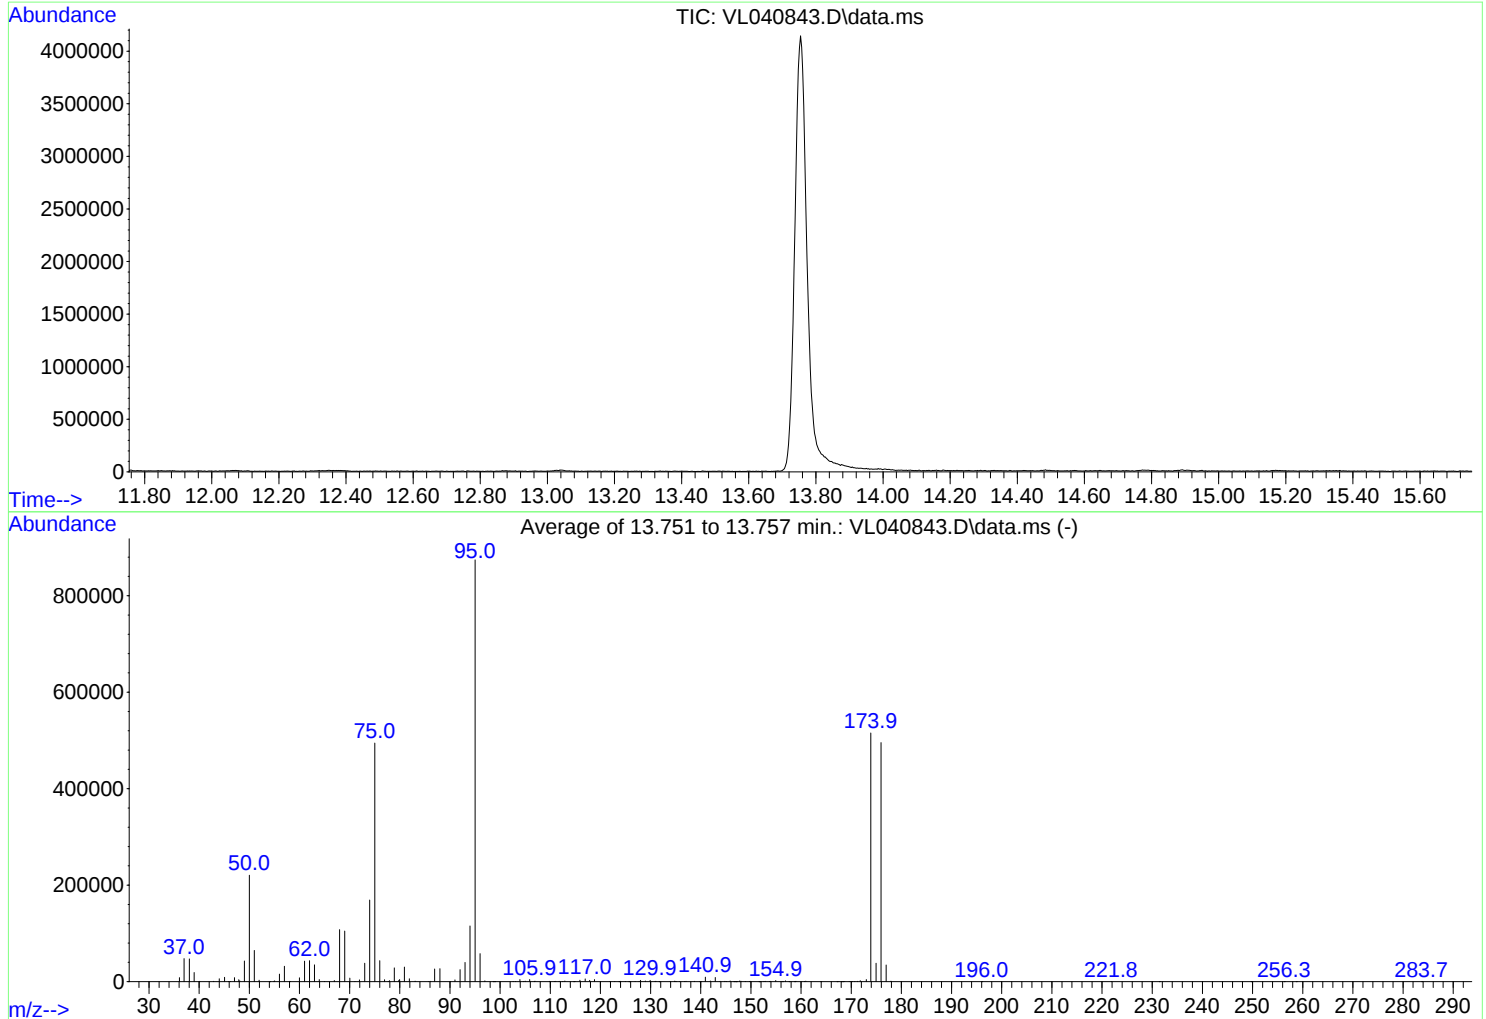

AutoFind: Scans 3467, 3468, 3469; Background Corrected with Scan 3441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.2	220587	PASS
75	95	30	66	56.5	494443	PASS
95	95	100	100	100.0	874347	PASS
96	95	5	9	6.6	58109	PASS
173	174	0.00	2	0.9	4473	PASS
174	95	50	120	58.9	515307	PASS
175	174	4	9	7.4	38325	PASS
176	174	93	101	96.2	495595	PASS
177	176	5	9	6.9	34387	PASS

Average of 13.751 to 13.757 min.: VL040843.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8385	47.90	3957	58.00	831	70.05	738
37.00	47677	48.10	1508	58.20	292	71.05	35
38.05	46963	49.00	42672	60.00	7811	71.95	370
39.00	18919	50.00	220587	61.00	42491	73.00	3802
40.10	767	51.00	64645	62.00	43384	74.00	169024
42.90	831	51.95	2997	63.00	34728	75.00	494443
44.00	6063	54.05	175	63.95	4305	76.00	43643
45.05	9030	54.90	640	65.00	413	76.95	4054
45.90	248	55.05	1851	66.95	2476	77.70	758
46.25	472	56.00	15689	68.00	107757	77.95	1874
47.05	8439	57.00	31856	69.00	104968	78.90	28683

Average of 13.751 to 13.757 min.: VL040843.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.80	2191	92.00	24963	104.70	474	114.65	100
79.95	4507	93.00	39888	105.00	911	114.95	382
80.90	30181	94.00	115349	105.90	4450	115.90	3078
81.90	5874	95.00	874347	106.80	306	116.95	5655
83.05	944	96.00	58109	106.95	903	117.85	2657
85.80	195	96.95	1803	109.80	595	118.80	4185
86.15	517	98.60	52	110.80	460	121.90	234
86.95	26088	98.90	103	111.10	564	122.85	368
88.00	27059	102.60	233	111.75	671	123.70	112
90.10	224	103.05	270	112.50	218	124.00	616
91.00	3573	103.95	4206	112.90	1203	124.95	468

Average of 13.751 to 13.757 min.: VL040843.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.65	181	134.75	892	142.90	8683	149.70	466
126.00	284	134.90	586	143.85	637	149.95	643
126.90	445	135.10	264	144.80	541	151.60	68
127.70	862	135.80	389	145.10	204	151.80	87
128.00	2621	136.80	497	145.85	1374	152.60	216
128.95	1219	137.05	647	146.60	118	152.85	564
129.90	2698	138.70	515	146.90	106	153.70	225
130.90	542	139.80	165	147.10	113	153.90	557
131.05	767	140.05	485	147.75	1188	154.95	2277
131.70	115	140.90	9193	148.00	1048	156.00	303
133.90	332	141.90	1235	148.90	405	156.30	86

Average of 13.751 to 13.757 min.: VL040843.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.90	1505	168.70	196	176.95	34387		
157.60	80	169.60	356	177.90	870		
158.70	173	169.90	394	196.00	63		
158.95	744	170.25	423	221.85	271		
160.70	243	170.70	199	231.40	74		
160.95	1046	171.20	757	249.70	72		
163.90	58	171.80	2083	256.30	81		
167.15	123	173.00	4473	258.70	51		
167.55	220	173.90	515307	283.70	56		
168.00	75	174.95	38325				
168.30	111	175.95	495595				