


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL111523\
 Data File : VL040864.D
 Acq On : 15 Nov 2023 10:14
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111323AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Nov 20 03:50:24 2023

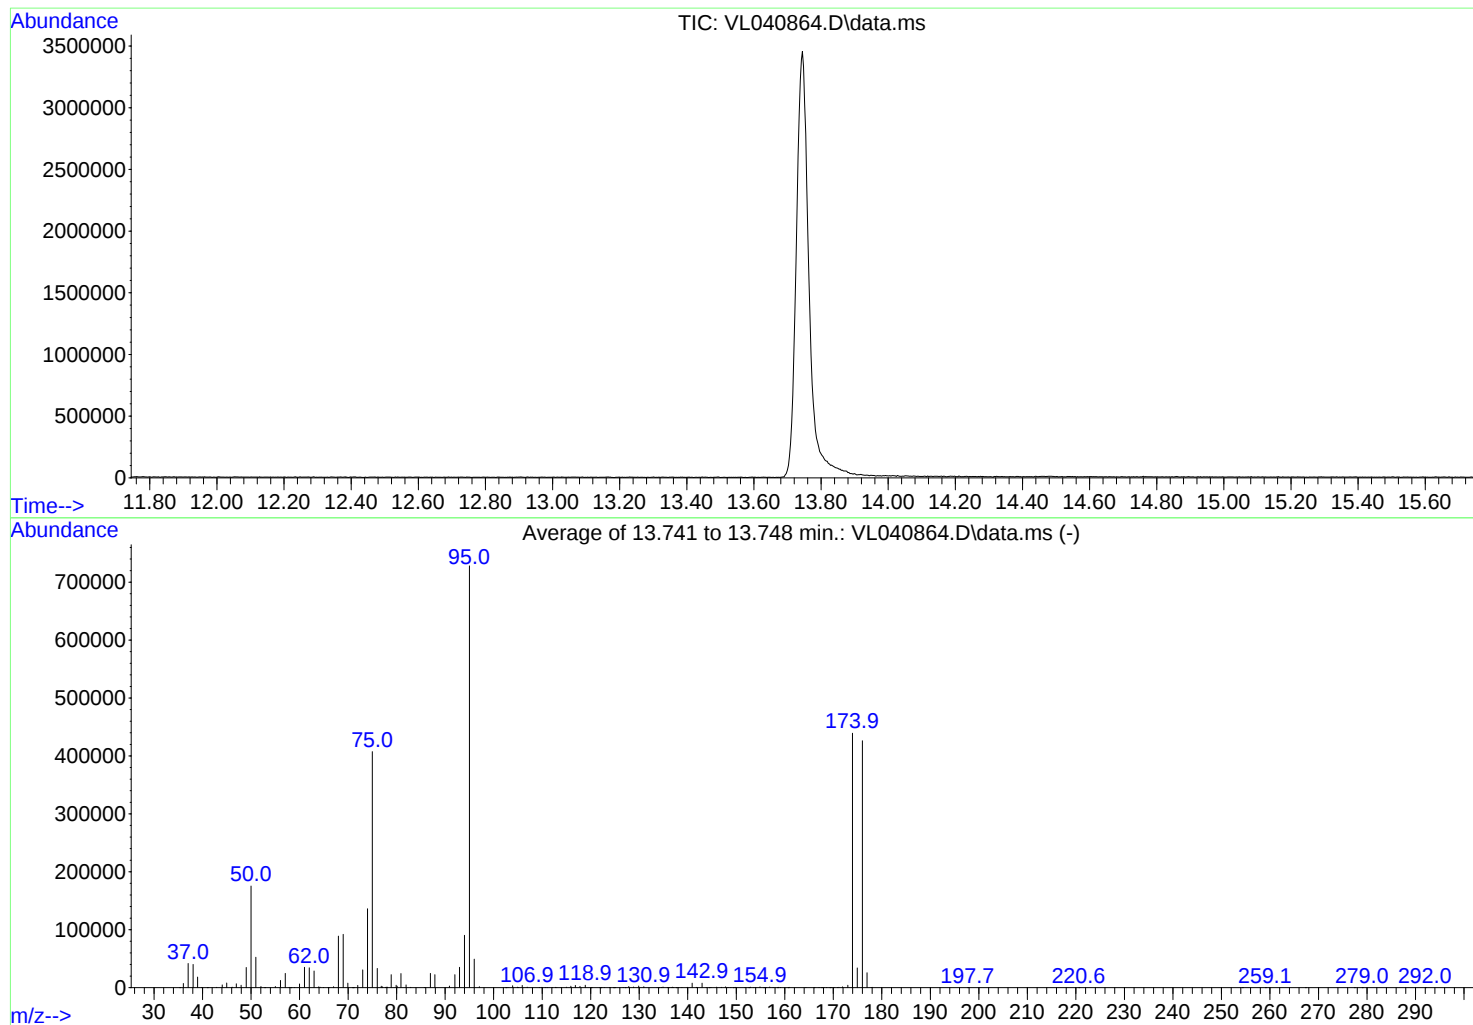

AutoFind: Scans 3464, 3465, 3466; Background Corrected with Scan 3435

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.1	175509	PASS
75	95	30	66	56.0	407488	PASS
95	95	100	100	100.0	728235	PASS
96	95	5	9	6.8	49267	PASS
173	174	0.00	2	0.9	4042	PASS
174	95	50	120	60.3	439264	PASS
175	174	4	9	7.8	34053	PASS
176	174	93	101	97.0	426197	PASS
177	176	5	9	6.1	25829	PASS

Average of 13.741 to 13.748 min.: VL040864.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.30	99	46.95	6681	58.00	213	67.00	163
36.05	7353	47.95	4266	58.20	142	68.00	8905
37.05	41800	49.00	34712	58.95	182	69.00	9208
38.05	40045	50.00	175509	60.00	6255	69.95	778
39.00	18318	51.00	52621	61.00	35107	70.90	79
39.85	376	52.05	1866	62.00	34184	71.10	69
41.00	105	52.80	79	63.00	28824	72.00	3821
42.90	509	55.00	2095	63.95	1508	73.00	30813
44.05	4660	56.05	12356	64.20	803	74.00	136256
45.00	8047	57.05	24563	64.95	367	75.00	407488
46.10	784	57.85	536	65.90	52	76.00	33221

Average of 13.741 to 13.748 min.: VL040864.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.85	2539	85.70	273	102.50	51	112.10	327
77.10	1535	85.90	310	102.95	289	112.75	521
77.70	595	86.95	24581	103.90	3341	113.00	168
77.90	727	87.90	22427	104.90	893	113.90	184
78.10	712	90.90	2896	105.10	367	115.00	844
78.90	22309	92.00	22395	105.90	3771	115.90	2415
79.90	4137	92.95	35128	106.90	892	116.85	3896
80.10	2517	94.00	90320	109.50	177	117.80	2220
80.90	24195	95.00	728235	109.95	507	118.90	4164
81.95	4596	96.00	49267	110.65	345	120.10	128
82.90	482	97.05	1579	111.05	380	121.90	92

Average of 13.741 to 13.748 min.: VL040864.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.10	73	129.90	2823	137.65	146	145.95	852
122.80	316	130.95	1697	138.15	187	146.95	551
123.90	280	133.70	250	138.80	265	147.80	1489
124.05	200	134.00	62	139.90	457	148.30	205
124.70	56	134.60	167	140.90	7723	148.90	367
124.90	53	134.90	1037	141.80	493	149.40	108
125.15	277	135.80	209	142.00	343	149.80	480
126.70	184	136.00	75	142.95	7799	151.80	292
127.10	125	136.60	219	143.80	219	152.60	96
127.85	1849	136.85	959	144.40	82	152.90	751
128.85	1125	137.10	364	144.80	432	153.65	391

Average of 13.741 to 13.748 min.: VL040864.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.05	361	164.35	210	171.90	1388	259.05	118
154.90	1371	166.00	57	173.00	4042	267.30	61
155.65	138	167.05	358	173.95	439264	277.40	102
156.00	86	167.60	90	174.95	34053	279.00	155
156.90	1205	168.10	284	176.00	426197	292.00	56
157.60	176	168.65	162	176.95	25829		
158.50	60	169.30	125	177.80	297		
158.70	546	169.70	203	178.00	702		
159.10	206	170.15	392	197.70	53		
160.70	151	170.90	347	220.60	147		
160.90	449	171.15	665	254.30	57		