


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL111723\
 Data File : VL040887.D
 Acq On : 17 Nov 2023 9:20
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111323AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Nov 20 03:50:24 2023

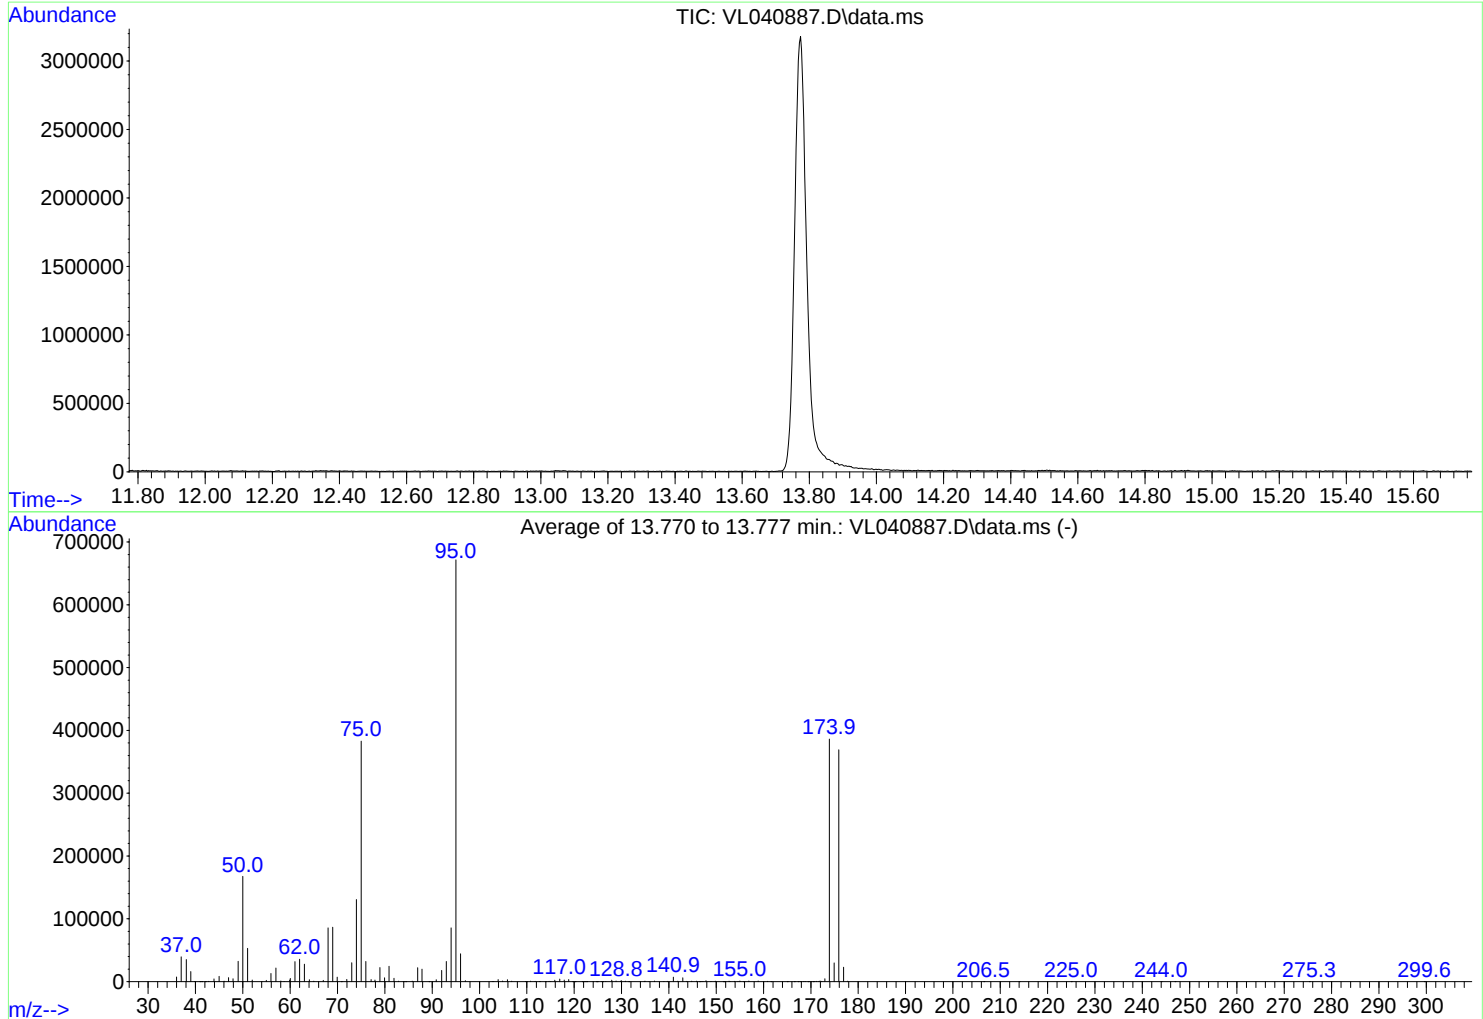

AutoFind: Scans 3473, 3474, 3475; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.0	167616	PASS
75	95	30	66	57.0	382891	PASS
95	95	100	100	100.0	671573	PASS
96	95	5	9	6.6	44427	PASS
173	174	0.00	2	1.2	4547	PASS
174	95	50	120	57.5	386155	PASS
175	174	4	9	7.7	29720	PASS
176	174	93	101	95.6	369067	PASS
177	176	5	9	6.2	23037	PASS

Average of 13.770 to 13.777 min.: VL040887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	7482	46.05	758	58.05	970	68.00	8570
37.00	39411	47.00	6450	58.70	225	69.00	8673
38.05	35211	47.95	4518	59.90	2540	69.95	718
39.00	15969	49.00	32475	60.05	5105	70.80	10
39.85	404	50.00	167616	61.00	31899	71.95	3510
40.95	118	51.00	52896	62.00	35592	73.00	30029
41.30	59	52.00	2607	63.00	27864	74.00	130731
42.10	53	54.05	260	64.05	3066	75.00	382891
42.80	418	54.95	2026	65.00	698	76.00	32227
43.90	4473	55.95	12898	66.00	222	77.10	3424
45.00	8288	57.00	21701	67.00	2063	77.90	2525

Average of 13.770 to 13.777 min.: VL040887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	22515	90.85	3071	105.90	3122	115.90	2310
79.95	6235	92.00	17911	106.80	775	116.95	4123
80.90	24435	93.00	32104	109.70	194	117.90	2475
81.95	5342	94.00	85517	109.90	129	118.85	3217
82.90	840	95.00	671573	110.80	784	119.70	98
83.90	57	96.00	44427	111.75	628	120.20	63
84.40	55	97.00	1473	112.65	313	121.70	54
85.80	810	102.70	254	112.90	191	122.20	54
86.95	22219	103.00	162	113.90	84	122.60	86
87.85	19997	103.95	3208	114.70	449	122.80	245
89.35	138	104.90	1144	115.05	351	124.00	372

Average of 13.770 to 13.777 min.: VL040887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.70	105	134.00	347	144.85	711	152.70	706
124.90	87	134.80	564	145.85	690	152.90	207
125.75	354	134.95	875	146.50	73	153.85	427
126.00	128	135.80	183	146.95	222	154.60	294
126.70	300	136.95	1085	147.20	241	155.00	1157
127.95	2298	138.95	361	147.85	1530	155.80	51
128.85	1035	139.65	554	148.90	337	156.90	1060
129.80	763	140.95	7126	149.80	686	158.85	1009
129.95	1504	141.90	695	151.50	135	160.85	639
130.80	687	142.95	6096	151.70	138	161.55	106
131.50	114	143.80	655	151.95	239	165.00	89

Average of 13.770 to 13.777 min.: VL040887.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
166.50	70	171.70	518	225.00	58		
167.30	56	171.95	1038	244.00	60		
167.80	67	172.30	594	246.90	53		
168.50	381	172.95	4547	275.30	127		
168.80	304	173.90	386155	299.60	56		
169.40	98	174.90	29720				
169.80	301	175.90	369067				
170.15	249	176.90	23037				
170.50	58	177.80	753				
170.70	185	206.50	95				
171.15	528	214.00	78				

Instrument :

MSVOA_L

ClientSampleId :

BFB